




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
 Data File : VW025451.D
 Acq On : 20 Mar 2023 18:25
 Operator : SY/MD
 Sample : 01979-10
 Misc : 6.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB5

Manual IntegrationsAPPROVED

Quant Time: Mar 20 23:55:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Mar 20 23:49:37 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/21/2023
 Supervised By :Mahesh Dadoda 03/21/2023

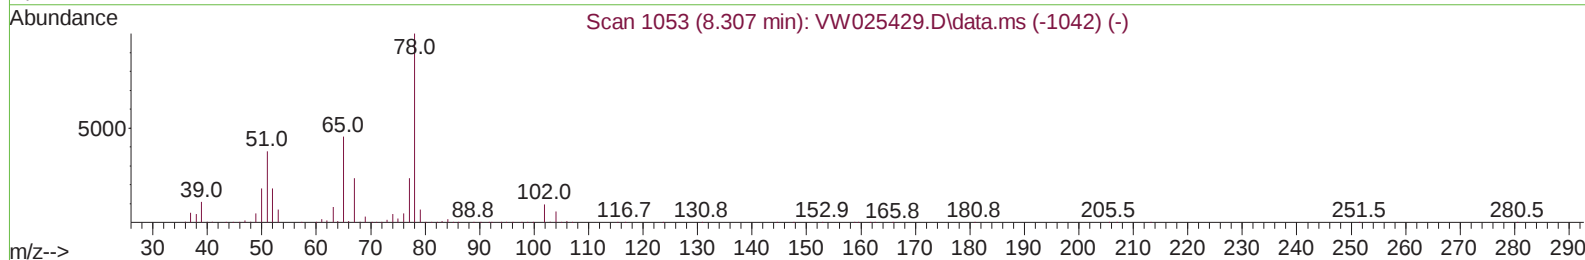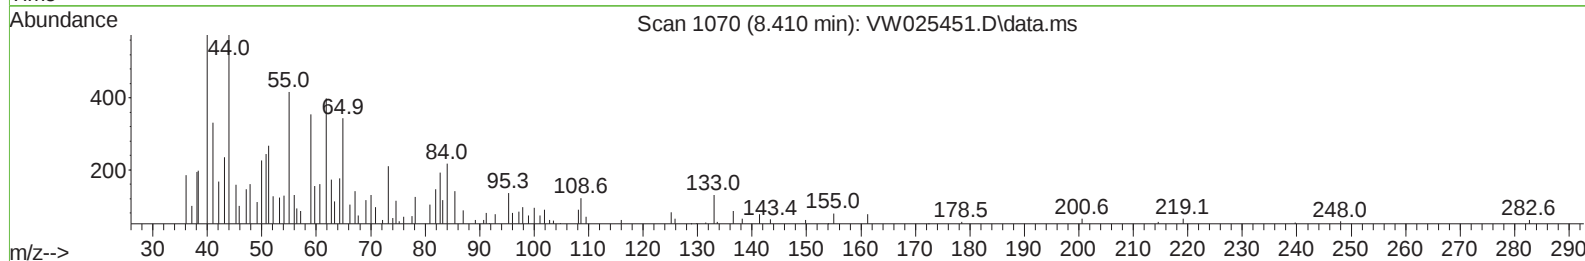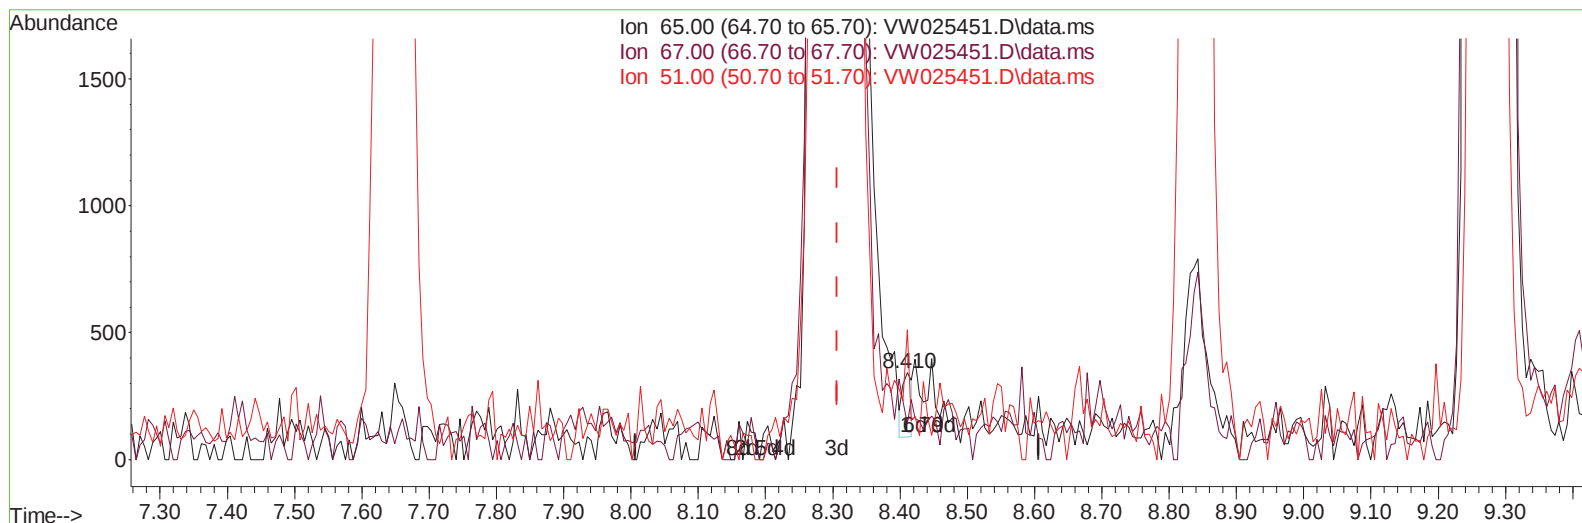

TIC: VW025451.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.410min (+ 0.104) 0.01 ug/L

response 250

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.30	40.40
51.00	111.10	82.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
 Data File : VW025451.D
 Acq On : 20 Mar 2023 18:25
 Operator : SY/MD
 Sample : 01979-10
 Misc : 6.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB5

Manual IntegrationsAPPROVED

Quant Time: Mar 20 23:55:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Mar 20 23:49:37 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/21/2023
 Supervised By :Mahesh Dadoda 03/21/2023

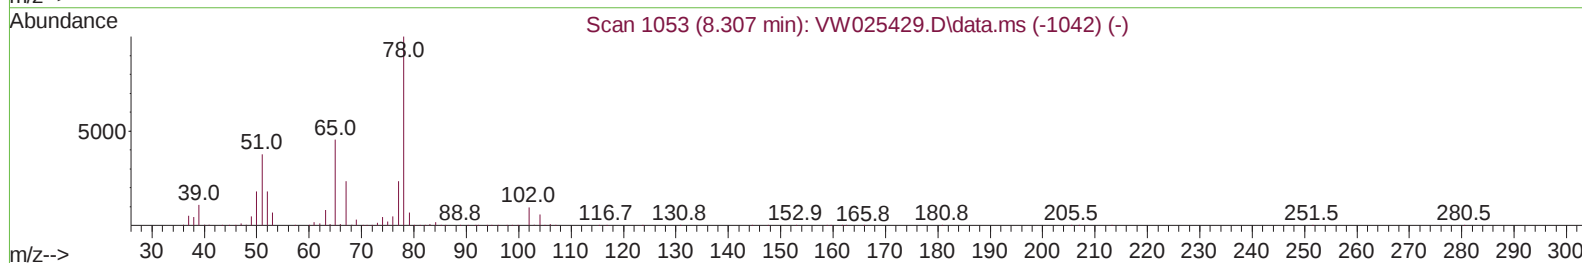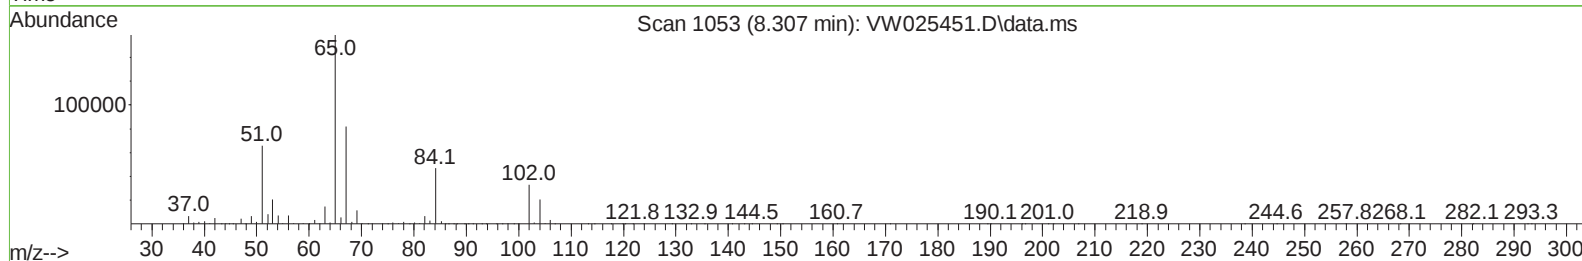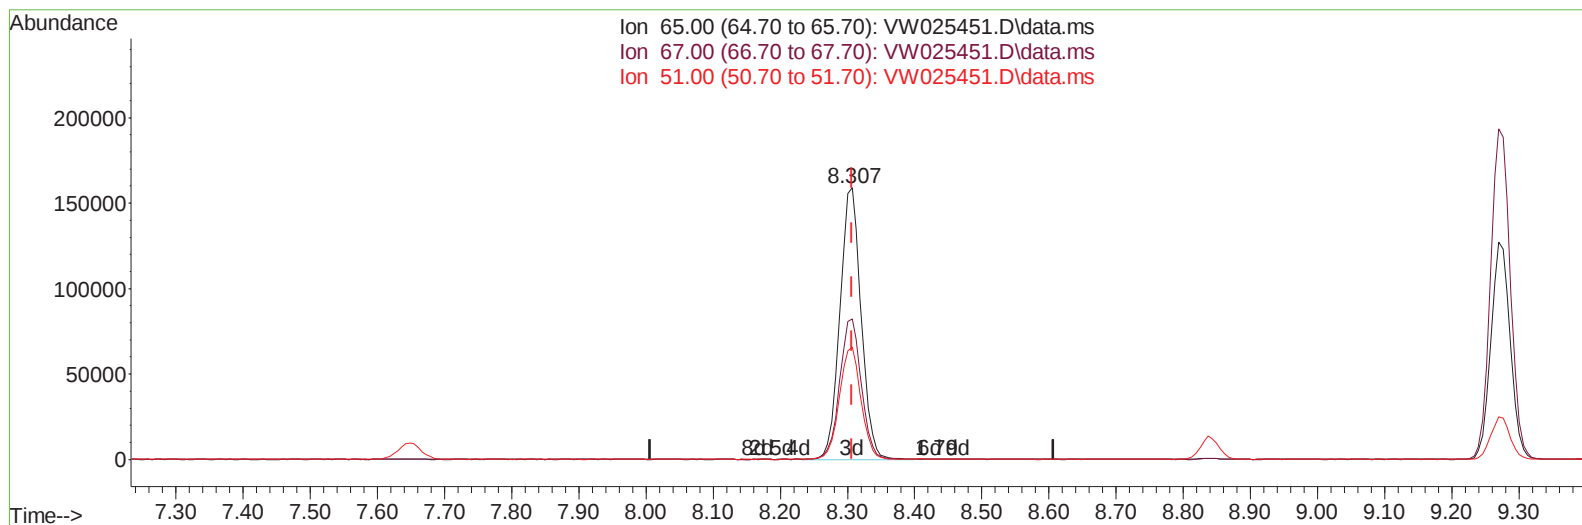

TIC: VW025451.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 20.24 ug/L m

response 348141

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.30	0.03#
51.00	111.10	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
 Data File : VW025451.D
 Acq On : 20 Mar 2023 18:25
 Operator : SY/MD
 Sample : 01979-10
 Misc : 6.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB5

Manual IntegrationsAPPROVED

Quant Time: Mar 20 23:55:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Mar 20 23:49:37 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/21/2023
 Supervised By :Mahesh Dadoda 03/21/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1111592	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	1006542	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	474381	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	173938	9.411	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	37.640%	
7) Chloroethane-d5	2.893	69	171700	12.911	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	51.640%	
11) 1,1-Dichloroethene-d2	4.021	63	380034	10.646	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	42.600%#	
21) 2-Butanone-d5	7.075	46	232190	51.181	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	102.360%	
24) Chloroform-d	7.648	84	569922	17.785	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	71.120%	
26) 1,2-Dichloroethane-d4	8.307	65	348141m	20.241	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	80.960%	
32) Benzene-d6	8.276	84	1175322	17.089	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	68.360%	
36) 1,2-Dichloropropane-d6	9.270	67	394957	18.563	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	74.240%	
41) Toluene-d8	10.325	98	1063062	17.531	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	70.120%	
43) trans-1,3-Dichloroprop...	10.575	79	160350	18.926	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	75.720%	
47) 2-Hexanone-d5	10.922	63	158487	51.801	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	103.600%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	349553	22.425	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	89.680%	
66) 1,2-Dichlorobenzene-d4	13.848	152	333547	18.907	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	75.640%	
Target Compounds						
13) Acetone	4.118	43	164694	37.764	ug/L	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
Data File : VW025451.D
Acq On : 20 Mar 2023 18:25
Operator : SY/MD
Sample : 01979-10
Misc : 6.69g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EYGB5

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 03/21/2023
Supervised By :Mahesh Dadoda 03/21/2023

Quant Time: Mar 20 23:55:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Mar 20 23:49:37 2023
Response via : Initial Calibration

