

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
 Data File : VW025443.D
 Acq On : 20 Mar 2023 15:13
 Operator : SY/MD
 Sample : 01979-01
 Misc : 3.97g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYG98

Quant Time: Mar 20 23:53:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Mar 20 23:49:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1095224	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	950659	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	398539	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	202204	11.104	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	44.400%
7) Chloroethane-d5	2.899	69	201953	15.413	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	61.640%
11) 1,1-Dichloroethene-d2	4.021	63	444196	12.629	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	50.520%
21) 2-Butanone-d5	7.075	46	281273	62.926	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	125.860%
24) Chloroform-d	7.648	84	667822	21.151	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.600%
26) 1,2-Dichloroethane-d4	8.307	65	405601	23.934	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.720%
32) Benzene-d6	8.276	84	1387318	21.357	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.440%
36) 1,2-Dichloropropane-d6	9.270	67	462475	23.014	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.040%
41) Toluene-d8	10.325	98	1215532	21.224	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.880%
43) trans-1,3-Dichloroprop...	10.575	79	189163	23.640	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.560%
47) 2-Hexanone-d5	10.922	63	193908	67.104	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	134.200%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	393900	26.755	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	107.040%
66) 1,2-Dichlorobenzene-d4	13.848	152	325298	21.949	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.800%
Target Compounds					Qvalue	
13) Acetone	4.119	43	75198	17.500	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
Data File : VW025443.D
Acq On : 20 Mar 2023 15:13
Operator : SY/MD
Sample : 01979-01
Misc : 3.97g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EYG98

Quant Time: Mar 20 23:53:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Mar 20 23:49:37 2023
Response via : Initial Calibration

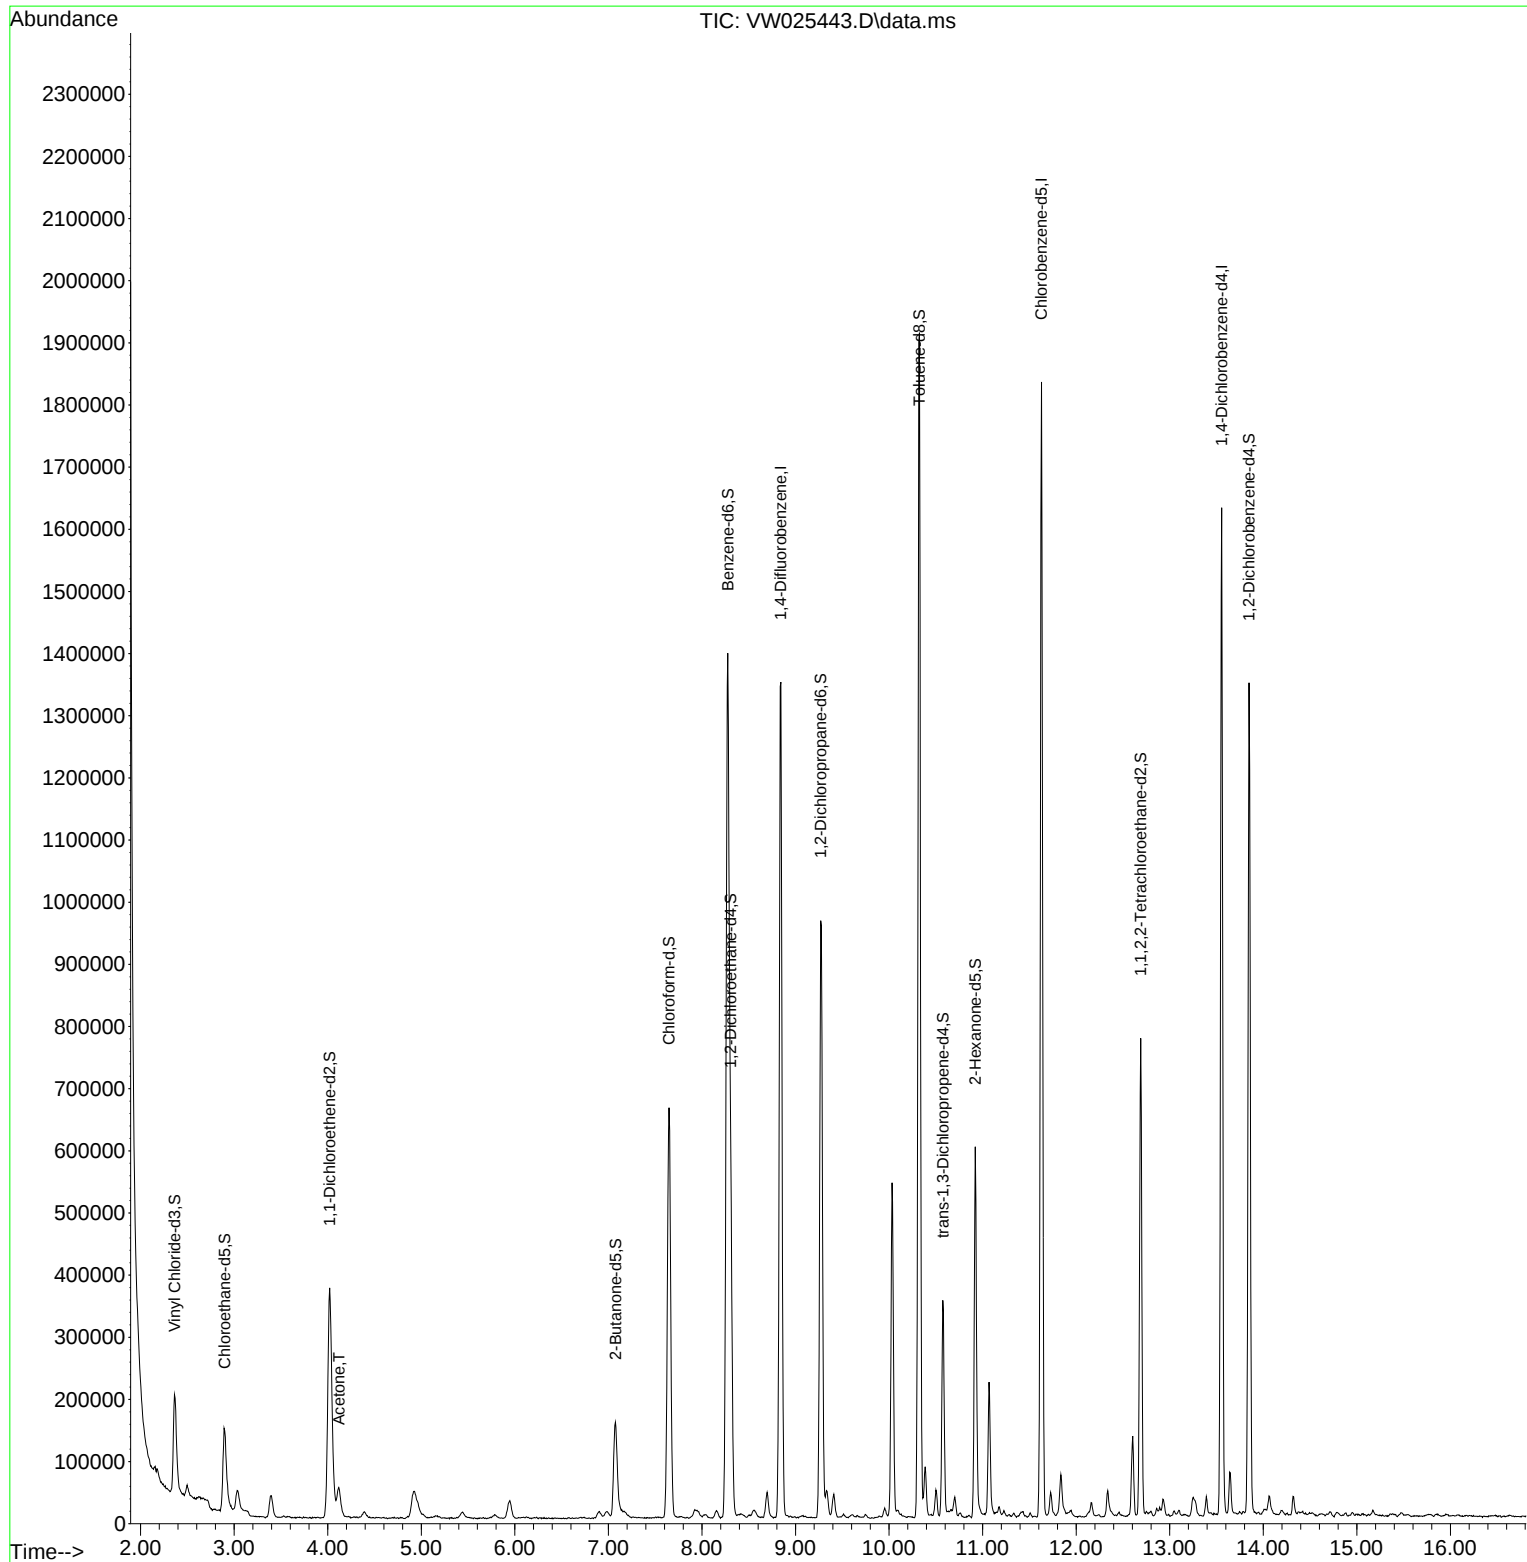

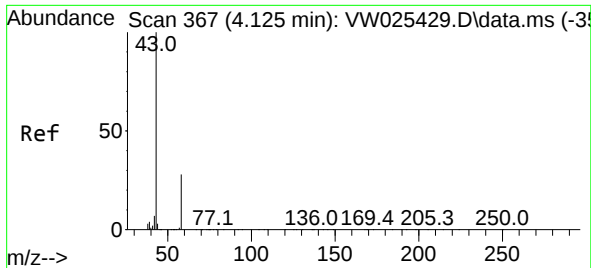

#13
 Acetone
 Concen: 17.500 ug/L
 RT: 4.119 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW025443.D
 Acq: 20 Mar 2023 15:13

Instrument :
 MSVOA_W
 ClientSampleId :
 EYG98

Tgt Ion: 43 Resp: 75198
 Ion Ratio Lower Upper
 43 100
 58 27.9 0.0 60.0

