

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
 Data File : VW025448.D
 Acq On : 20 Mar 2023 17:13
 Operator : SY/MD
 Sample : 01979-06
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB1

Quant Time: Mar 20 23:54:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Mar 20 23:49:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	718952	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	639292	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	269224	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	131856	11.030	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	44.120%	
7) Chloroethane-d5	2.899	69	126674	14.727	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	58.920%	
11) 1,1-Dichloroethene-d2	4.021	63	277268	12.009	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	48.040%	
21) 2-Butanone-d5	7.075	46	182410	62.167	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	124.340%	
24) Chloroform-d	7.648	84	395673	19.090	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	76.360%	
26) 1,2-Dichloroethane-d4	8.307	65	246234	22.134	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	88.520%	
32) Benzene-d6	8.276	84	806037	18.452	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	73.800%	
36) 1,2-Dichloropropane-d6	9.270	67	269373	19.933	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	79.720%	
41) Toluene-d8	10.325	98	699908	18.173	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	72.680%	
43) trans-1,3-Dichloroprop...	10.575	79	106689	19.827	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	79.320%	
47) 2-Hexanone-d5	10.922	63	121474	62.512	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	125.020%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	254562	25.712	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	102.840%	
66) 1,2-Dichlorobenzene-d4	13.848	152	207905	20.766	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	83.080%	
Target Compounds						
13) Acetone	4.125	43	45144	16.005	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
Data File : VW025448.D
Acq On : 20 Mar 2023 17:13
Operator : SY/MD
Sample : 01979-06
Misc : 5.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EYGB1

Quant Time: Mar 20 23:54:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Mar 20 23:49:37 2023
Response via : Initial Calibration

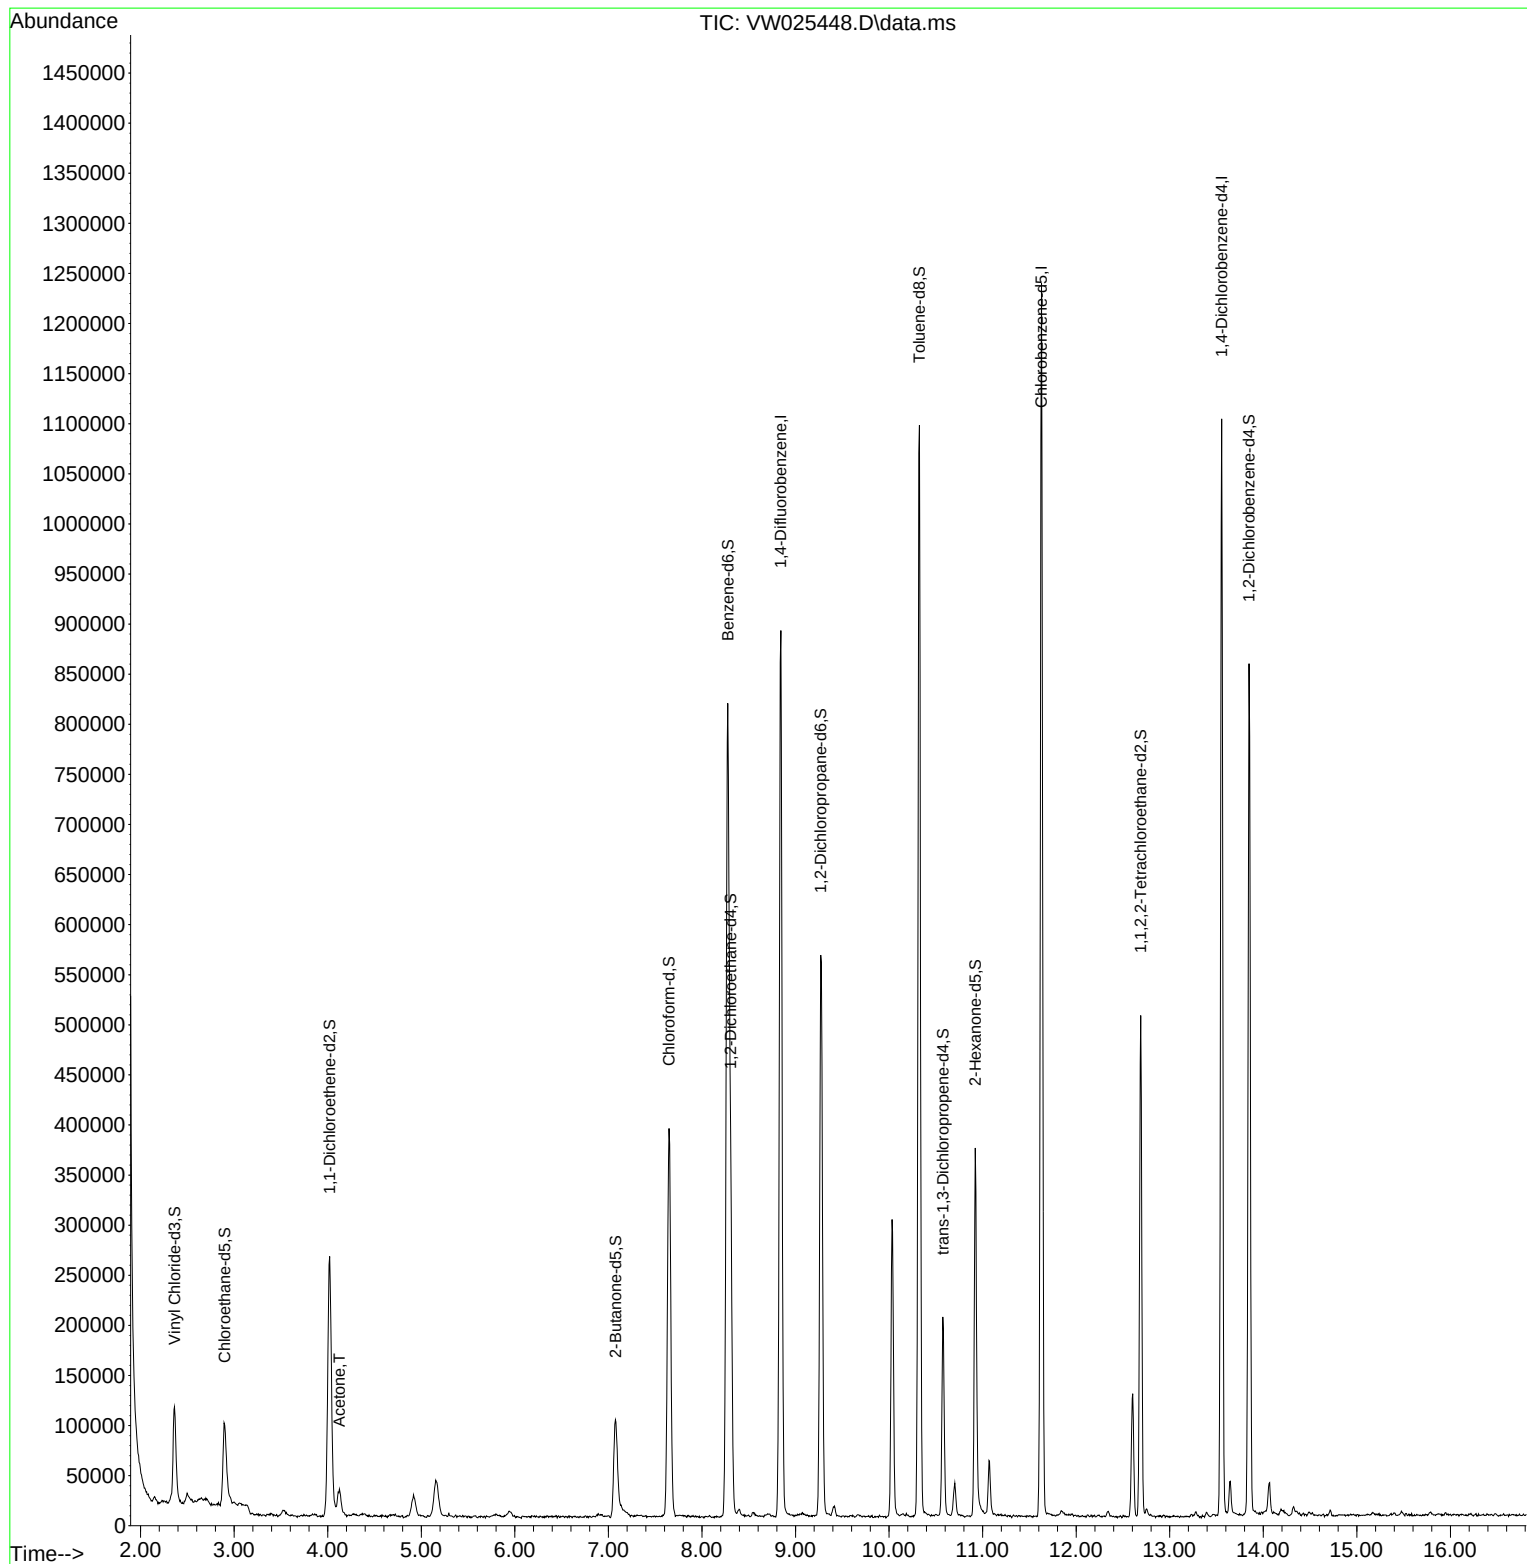

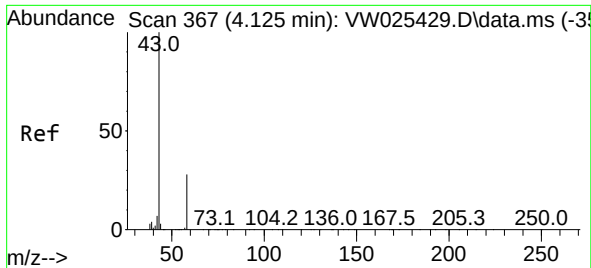

#13
 Acetone
 Concen: 16.005 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW025448.D
 Acq: 20 Mar 2023 17:13

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB1

Tgt Ion: 43 Resp: 45144
 Ion Ratio Lower Upper
 43 100
 58 28.6 0.0 60.0

