

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
 Data File : VW025449.D
 Acq On : 20 Mar 2023 17:37
 Operator : SY/MD
 Sample : 01979-07
 Misc : 3.17g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB2

Quant Time: Mar 20 23:54:50 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Mar 20 23:49:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	485983	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	450379	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	187873	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	102437	12.677	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	50.720%
7) Chloroethane-d5	2.899	69	97219	16.721	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.880%
11) 1,1-Dichloroethene-d2	4.015	63	214527	13.746	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.000%
21) 2-Butanone-d5	7.075	46	106438	53.664	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.320%
24) Chloroform-d	7.648	84	300027	21.415	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.640%
26) 1,2-Dichloroethane-d4	8.307	65	180910	24.058	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.240%
32) Benzene-d6	8.276	84	615855	20.012	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	80.040%
36) 1,2-Dichloropropane-d6	9.276	67	205355	21.570	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.280%
41) Toluene-d8	10.325	98	538613	19.851	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.400%
43) trans-1,3-Dichloroprop...	10.575	79	77066	20.329	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.320%
47) 2-Hexanone-d5	10.922	63	68486	50.027	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.060%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	172113	24.676	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.720%
66) 1,2-Dichlorobenzene-d4	13.848	152	158428	22.676	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.720%
Target Compounds						
13) Acetone	4.125	43	18745	9.831	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
Data File : VW025449.D
Acq On : 20 Mar 2023 17:37
Operator : SY/MD
Sample : 01979-07
Misc : 3.17g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EYGB2

Quant Time: Mar 20 23:54:50 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Mar 20 23:49:37 2023
Response via : Initial Calibration

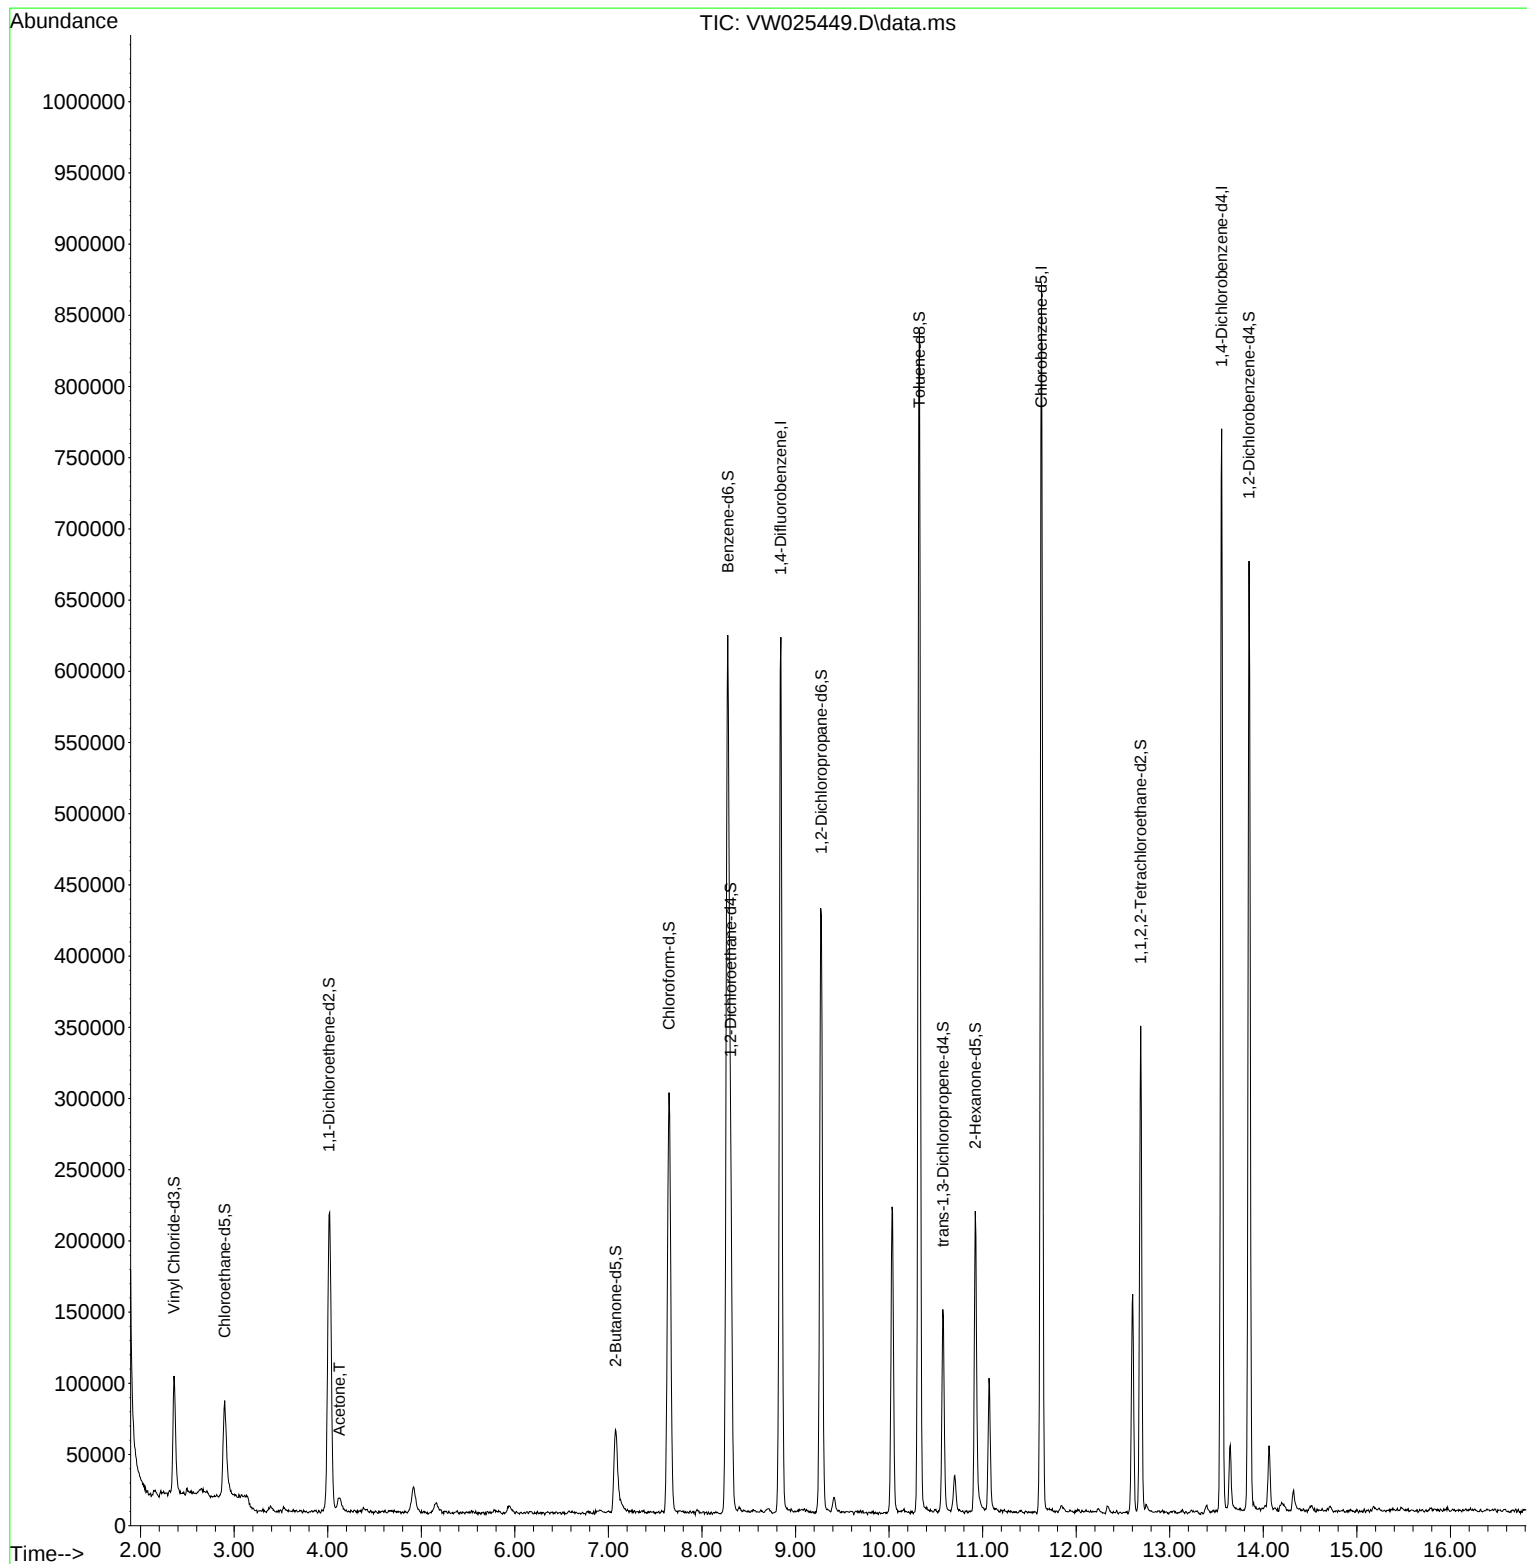

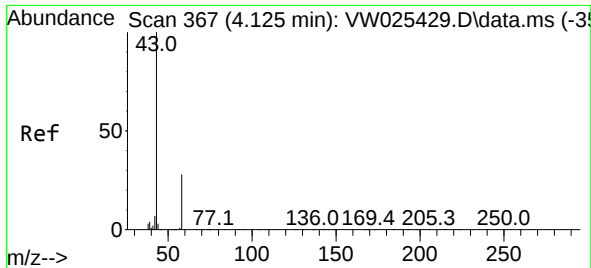

#13
 Acetone
 Concen: 9.831 ug/L
 RT: 4.125 min Scan# 3
 Delta R.T. -0.000 min
 Lab File: VW025449.D
 Acq: 20 Mar 2023 17:37

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB2

Tgt Ion: 43 Resp: 18745
 Ion Ratio Lower Upper
 43 100
 58 30.9 0.0 60.0

