

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
 Data File : VW025451.D
 Acq On : 20 Mar 2023 18:25
 Operator : SY/MD
 Sample : 01979-10
 Misc : 6.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB5

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 03/21/2023
 Supervised By :Mahesh Dadoda 03/21/2023

Quant Time: Mar 20 23:55:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Mar 20 23:49:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1111592	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	1006542	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	474381	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	173938	9.411	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	37.640%		
7) Chloroethane-d5	2.893	69	171700	12.911	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	51.640%		
11) 1,1-Dichloroethene-d2	4.021	63	380034	10.646	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery =	42.600%#		
21) 2-Butanone-d5	7.075	46	232190	51.181	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	102.360%		
24) Chloroform-d	7.648	84	569922	17.785	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery =	71.120%		
26) 1,2-Dichloroethane-d4	8.307	65	348141m	20.241	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery =	80.960%		
32) Benzene-d6	8.276	84	1175322	17.089	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery =	68.360%		
36) 1,2-Dichloropropane-d6	9.270	67	394957	18.563	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery =	74.240%		
41) Toluene-d8	10.325	98	1063062	17.531	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery =	70.120%		
43) trans-1,3-Dichloroprop...	10.575	79	160350	18.926	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery =	75.720%		
47) 2-Hexanone-d5	10.922	63	158487	51.801	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	103.600%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	349553	22.425	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery =	89.680%		
66) 1,2-Dichlorobenzene-d4	13.848	152	333547	18.907	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery =	75.640%		
Target Compounds					Qvalue	
13) Acetone	4.118	43	164694	37.764	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
Data File : VW025451.D
Acq On : 20 Mar 2023 18:25
Operator : SY/MD
Sample : 01979-10
Misc : 6.69g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EYGB5

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 03/21/2023
Supervised By :Mahesh Dadoda 03/21/2023


Quant Time: Mar 20 23:55:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Mar 20 23:49:37 2023
Response via : Initial Calibration

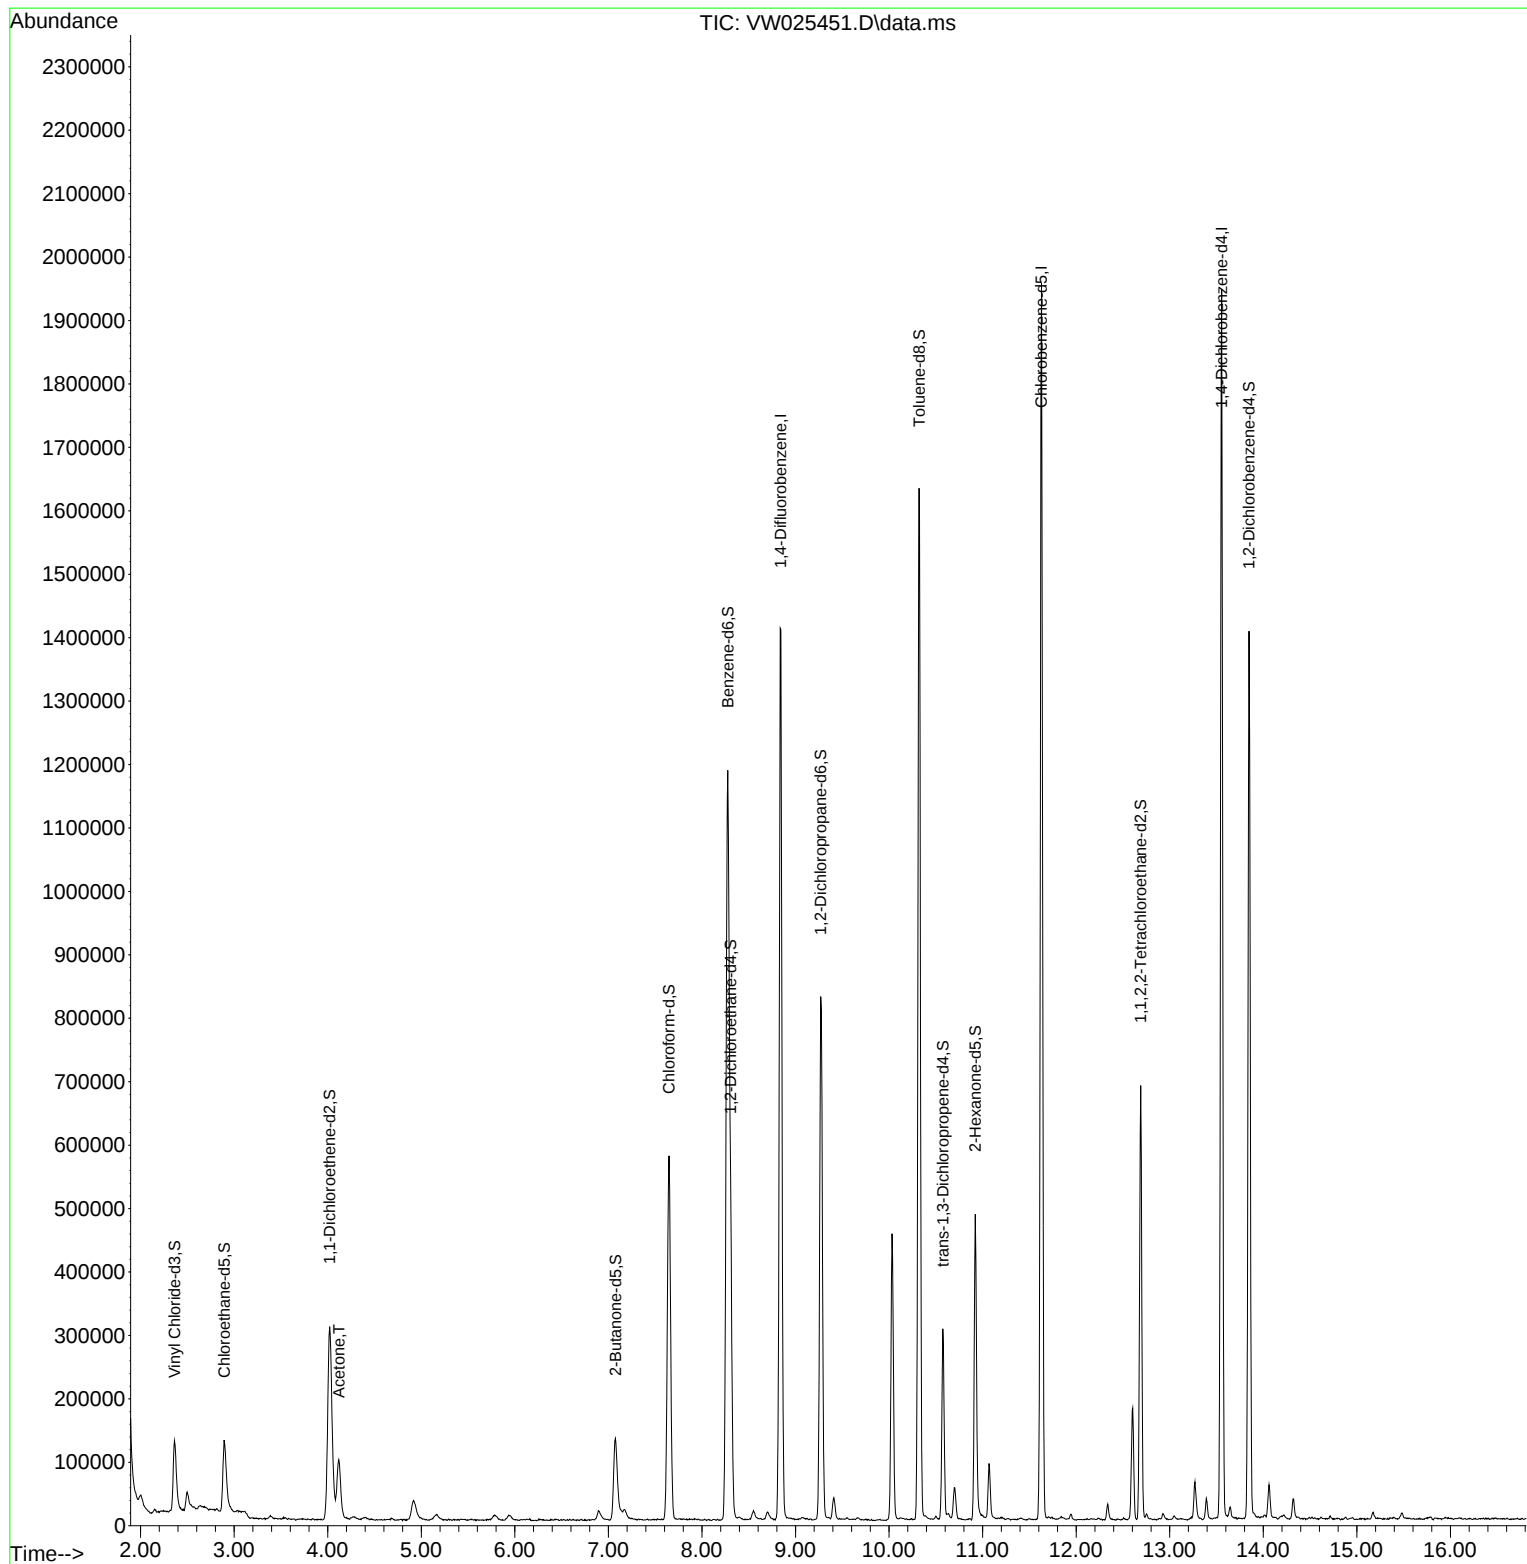

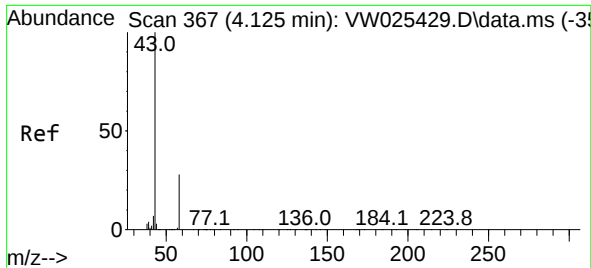

#13
 Acetone
 Concen: 37.764 ug/L
 RT: 4.118 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW025451.D
 Acq: 20 Mar 2023 18:25

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB5

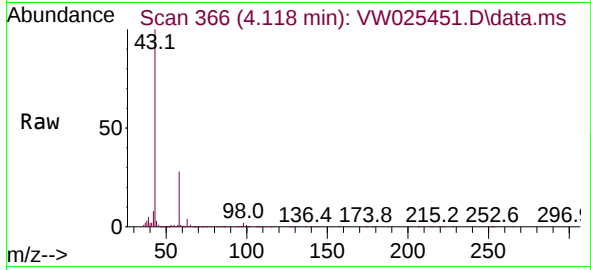

Tgt Ion: 43 Resp: 164694
 Ion Ratio Lower Upper
 43 100
 58 29.1 0.0 60.0

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 03/21/2023
 Supervised By :Mahesh Dadoda 03/21/2023

