

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032024\
 Data File : VW028214.D
 Acq On : 20 Mar 2024 12:58
 Operator : SY/MD
 Sample : P1812-02
 Misc : 4.17g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Mar 21 01:13:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 21 01:12:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	329512	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	270117	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	102152	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	60677	15.738	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.960%
7) Chloroethane-d5	2.905	69	44248	16.427	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.720%
11) 1,1-Dichloroethene-d2	4.027	65	42147	17.239	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.960%
21) 2-Butanone-d5	7.081	46	41340	36.355	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	72.700%
24) Chloroform-d	7.654	84	181116	18.640	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	74.560%
26) 1,2-Dichloroethane-d4	8.307	65	99644	18.609	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	74.440%
32) Benzene-d6	8.276	84	342554	20.771	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.080%
36) 1,2-Dichloropropane-d6	9.270	67	98823	20.823	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.280%
41) Toluene-d8	10.319	98	295945	19.455	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.840%
43) trans-1,3-Dichloroprop...	10.575	79	41771	19.378	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.520%
47) 2-Hexanone-d5	10.922	63	33039	42.116	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.240%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	66742	19.038	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	76.160%
66) 1,2-Dichlorobenzene-d4	13.849	152	75029	20.162	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	80.640%
Target Compounds						
39) cis-1,3-Dichloropropene	10.038	75	3365	0.494	ug/L	Qvalue # 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032024\
Data File : VW028214.D
Acq On : 20 Mar 2024 12:58
Operator : SY/MD
Sample : P1812-02
Misc : 4.17g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Mar 21 01:13:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 21 01:12:17 2024
Response via : Initial Calibration

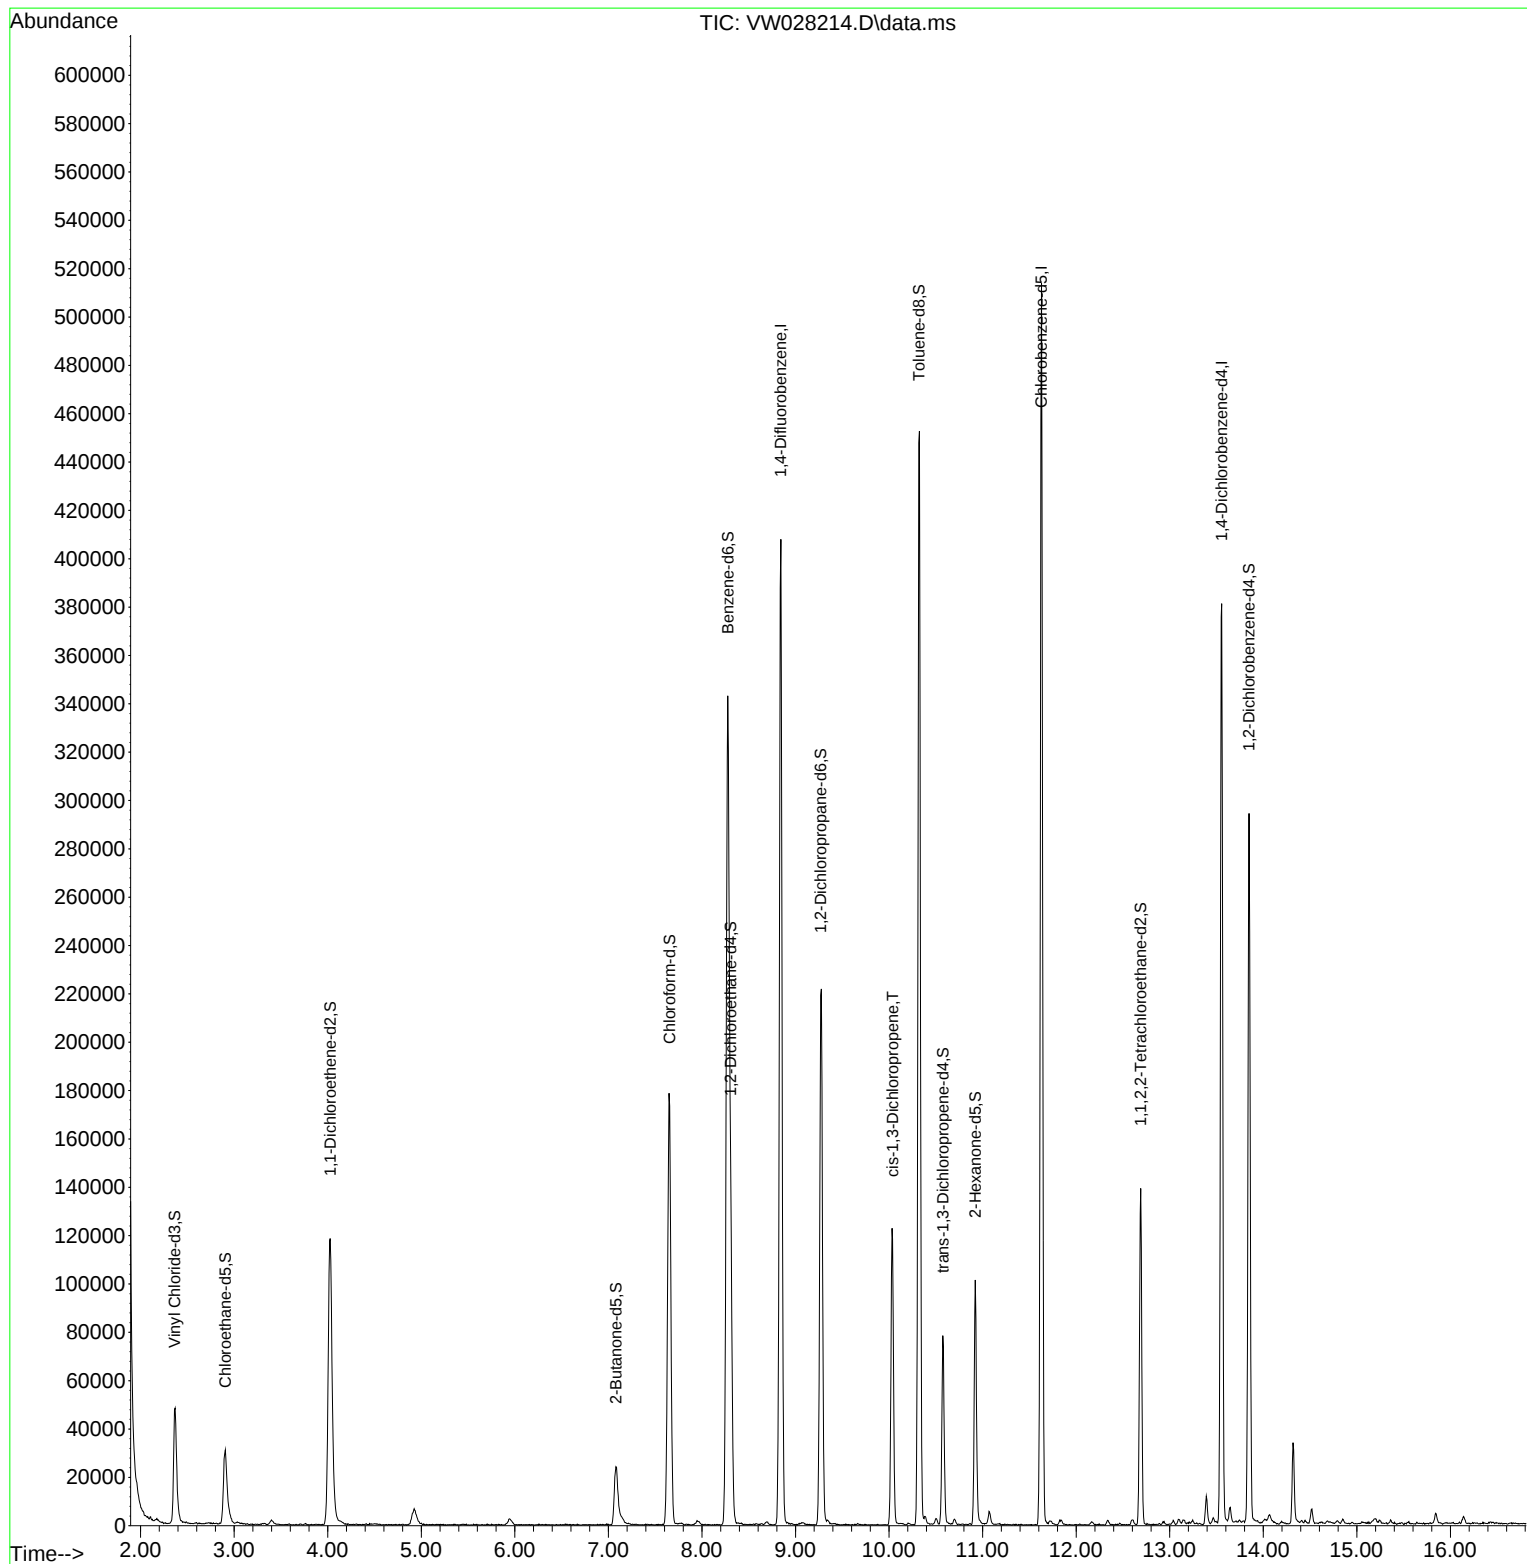

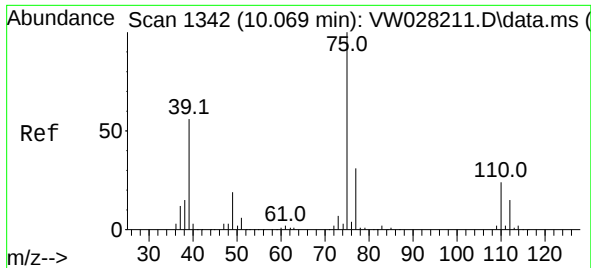

#39
 cis-1,3-Dichloropropene
 Concen: 0.494 ug/L
 RT: 10.038 min Scan# 14
 Delta R.T. -0.030 min
 Lab File: VW028214.D
 Acq: 20 Mar 2024 12:58

Instrument :
 MSVOA_W
 ClientSampleId :

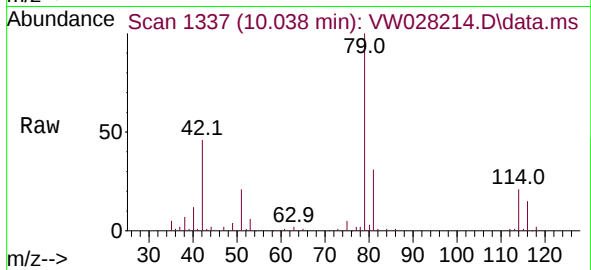

Tgt Ion: 75 Resp: 3365
 Ion Ratio Lower Upper
 75 100
 77 50.4 22.5 41.7#

