

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032024\
 Data File : VW028217.D
 Acq On : 20 Mar 2024 14:10
 Operator : SY/MD
 Sample : P1812-05
 Misc : 4.36g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Mar 21 01:14:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 21 01:12:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	356965	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	307879	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	131195	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	58508	14.008	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	56.040%		
7) Chloroethane-d5	2.899	69	43932	15.055	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	60.240%		
11) 1,1-Dichloroethene-d2	4.027	65	40522	15.299	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	61.200%		
21) 2-Butanone-d5	7.081	46	44425	36.063	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	72.120%		
24) Chloroform-d	7.648	84	182791	17.366	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	69.480%		
26) 1,2-Dichloroethane-d4	8.447	65	77	0.013	ug/L	0.15
Spiked Amount 25.000	Range 70 - 130		Recovery =	0.040%#		
32) Benzene-d6	8.276	84	343457	18.272	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	73.080%		
36) 1,2-Dichloropropane-d6	9.270	67	101940	18.845	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	75.360%		
41) Toluene-d8	10.318	98	303274	17.492	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	69.960%		
43) trans-1,3-Dichloroprop...	10.575	79	43083	17.536	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	70.160%		
47) 2-Hexanone-d5	10.922	63	36234	40.523	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	81.040%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	75552	18.908	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	75.640%		
66) 1,2-Dichlorobenzene-d4	13.848	152	89210	18.666	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	74.680%#		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3406	0.439	ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032024\
Data File : VW028217.D
Acq On : 20 Mar 2024 14:10
Operator : SY/MD
Sample : P1812-05
Misc : 4.36g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Mar 21 01:14:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 21 01:12:17 2024
Response via : Initial Calibration

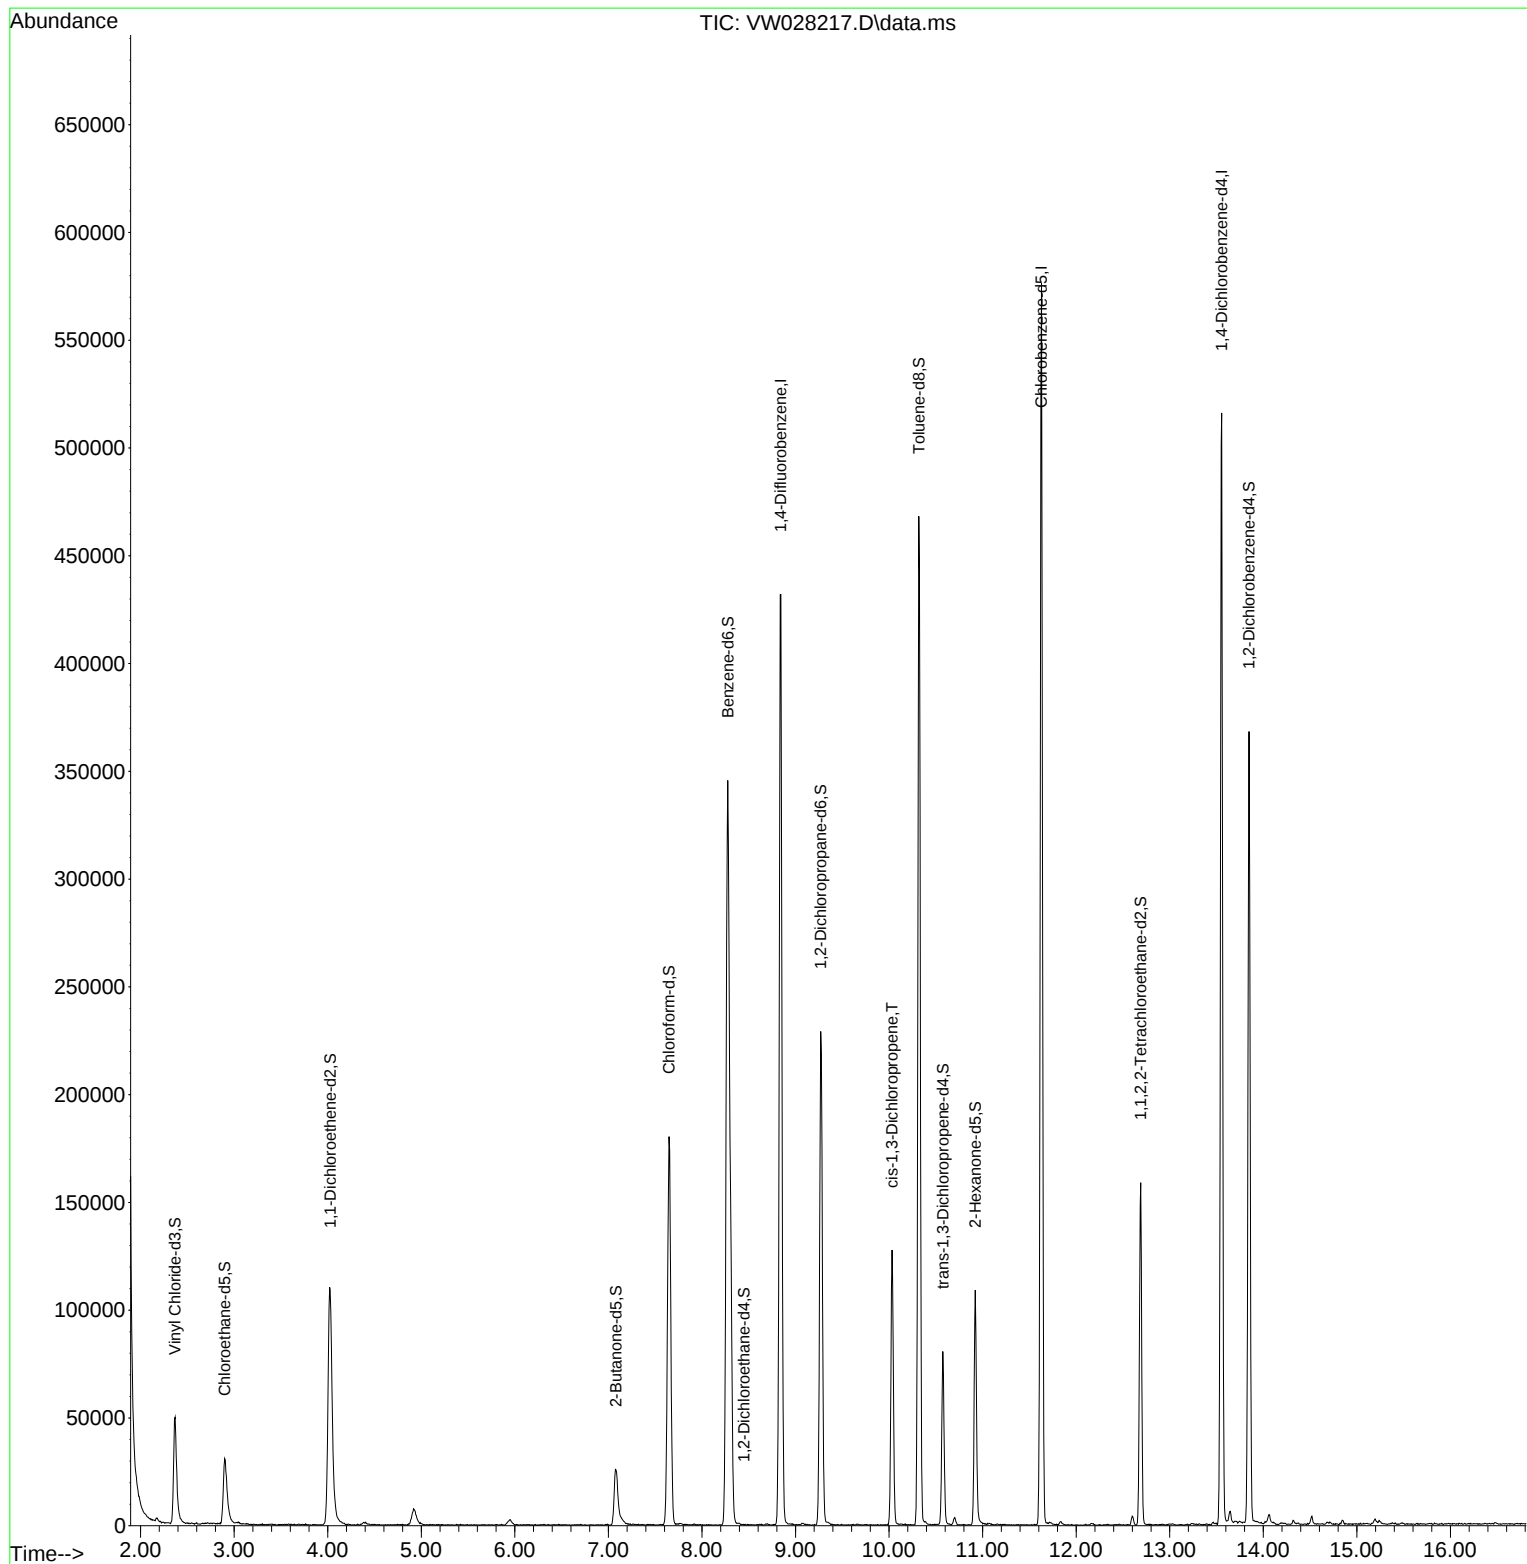

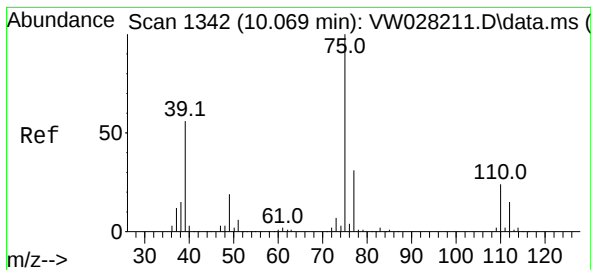

#39
 cis-1,3-Dichloropropene
 Concen: 0.439 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW028217.D
 Acq: 20 Mar 2024 14:10

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3406
 Ion Ratio Lower Upper
 75 100
 77 50.1 22.5 41.7#

