
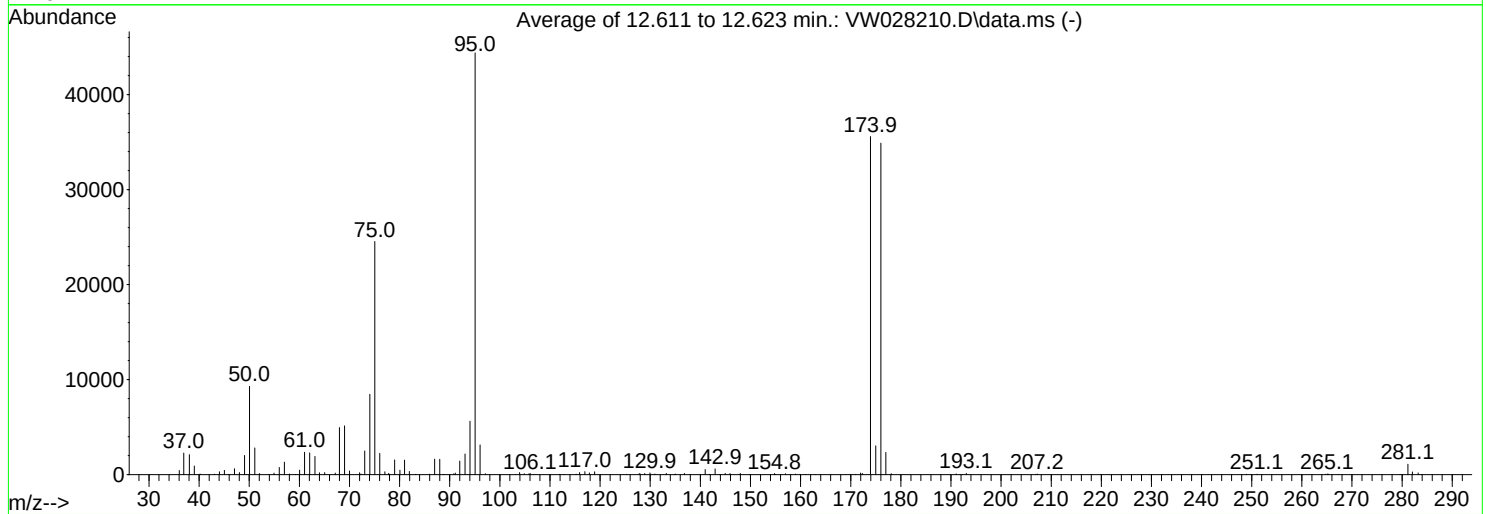


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032024\
Data File : VW028210.D
Acq On : 20 Mar 2024 09:57
Operator : SY/MD
Sample : BFB455
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB455

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Title : SFAM01.0
Last Update : Thu Mar 21 01:12:17 2024

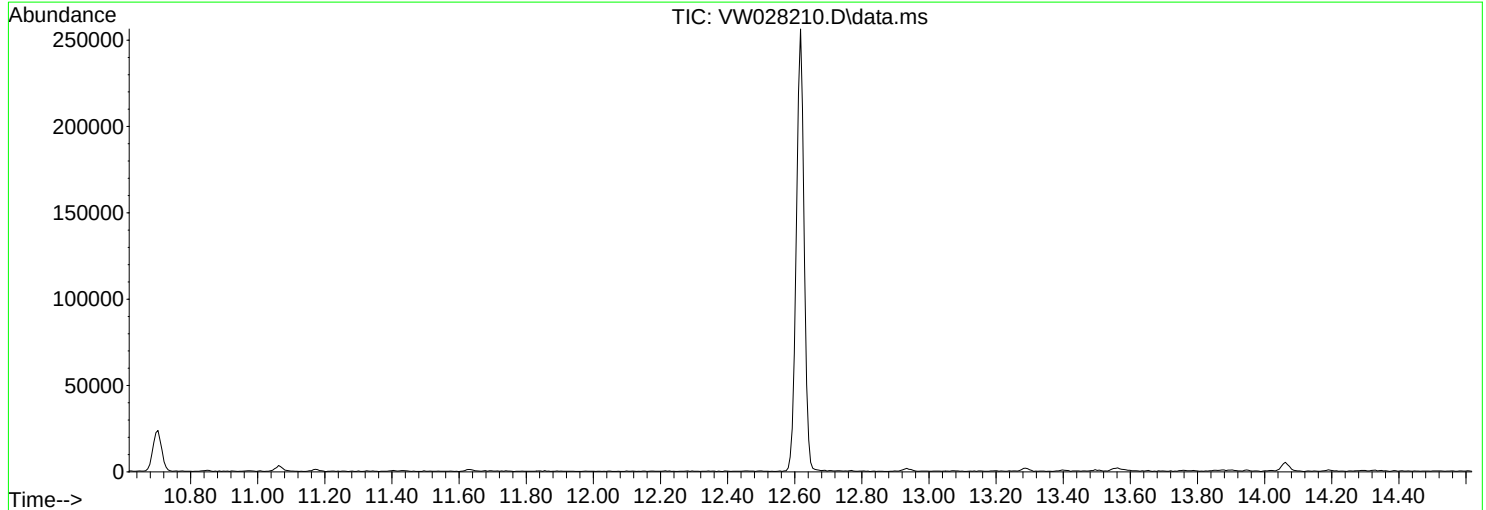

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	9302	PASS
75	95	30	80	55.3	24541	PASS
95	95	100	100	100.0	44395	PASS
96	95	5	9	7.0	3128	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.2	35592	PASS
175	174	5	9	8.5	3030	PASS
176	174	95	101	98.0	34893	PASS
177	176	5	9	6.7	2348	PASS

m/z	Abundance
36.90	74.0
38.50	77.0
40.00	183.0
41.20	72.0
43.70	50.0
44.20	103.0

Instrument :
MSVOA_W
ClientSampleId :
BFB455

m/z	Abundance
36.10	481.0
37.00	2653.0
38.00	2146.0
39.00	964.0
40.00	169.0
43.00	71.0
44.10	415.0
45.10	469.0
45.90	59.0
47.00	473.0
48.00	407.0
49.00	2016.0
50.10	9622.0
51.10	2913.0
52.00	144.0
54.90	137.0
56.00	693.0
57.00	1246.0
58.10	123.0
59.20	60.0
60.10	492.0
61.10	2431.0
62.00	2441.0
63.10	2032.0
63.90	178.0
65.00	260.0
67.20	170.0
68.00	4906.0
69.00	5258.0
70.00	472.0
72.00	294.0
73.10	2427.0
74.10	8342.0
75.00	24712.0
76.10	2201.0
77.00	320.0
77.90	202.0
79.00	1556.0
80.00	494.0
81.00	1551.0
81.90	335.0
83.20	66.0
87.00	1435.0
88.00	1587.0
91.20	245.0
92.00	1420.0
93.00	2146.0
94.10	5317.0
95.10	42896.0
96.00	3118.0
97.20	79.0
103.10	54.0
103.90	261.0
104.90	136.0
105.80	256.0
106.80	72.0
115.20	92.0
115.90	151.0
117.00	299.0
117.80	175.0
119.00	301.0
125.20	67.0
127.80	168.0
128.90	91.0
129.90	215.0
131.00	100.0
133.20	185.0
134.80	121.0
136.90	164.0
140.90	531.0
142.90	645.0
143.90	67.0
145.00	139.0
146.00	91.0
148.10	111.0
149.90	64.0
154.80	148.0
156.10	50.0
157.00	82.0
159.00	97.0
163.00	51.0
169.00	53.0
170.00	77.0
172.00	273.0
173.90	29960.0
175.00	2635.0
176.00	30480.0
177.00	2251.0
178.10	111.0
191.10	144.0
191.80	69.0
192.30	56.0

Instrument :
MSVOA_W
ClientSampleId :
BFB455

193.10	294.0
207.20	149.0
248.90	74.0
251.00	65.0
265.10	203.0
267.20	81.0
279.60	54.0
281.10	1557.0
282.10	516.0
283.20	247.0
283.90	53.0

Instrument :
MSVOA_W
ClientSampleId :
BFB455

m/z	Abundance
36.10	464.0
37.00	2647.0
38.10	2350.0
39.10	975.0
40.00	205.0
43.10	61.0
44.00	406.0
45.10	518.0
47.10	824.0
49.10	2289.0
50.00	10627.0
51.10	3005.0
52.10	102.0
55.00	228.0
56.00	869.0
57.00	1488.0
58.00	103.0
60.10	540.0
61.00	2712.0
62.00	2310.0
63.10	1914.0
64.00	227.0
65.00	215.0
67.10	163.0
68.00	5323.0
69.00	5527.0
70.00	468.0
72.00	317.0
73.00	2949.0
74.10	9012.0
75.00	27504.0
76.10	2475.0
77.00	271.0
77.70	153.0
79.00	1809.0
80.10	425.0
81.00	1614.0
82.00	347.0
83.10	61.0
86.00	97.0
87.00	1922.0
88.00	1874.0
88.80	80.0
90.80	243.0
92.00	1537.0
93.10	2425.0
94.10	6605.0
95.00	50496.0
96.00	3484.0
97.10	123.0
104.00	198.0
104.80	96.0
106.10	155.0
111.90	51.0
112.80	63.0
115.20	50.0
115.90	243.0
117.00	317.0
117.90	238.0
118.90	304.0
125.30	55.0
128.00	219.0
128.90	128.0
129.90	196.0
130.90	62.0
133.20	138.0
135.00	136.0
136.80	149.0
140.00	84.0
141.00	609.0
143.00	703.0
144.90	158.0
145.80	90.0
146.10	78.0
147.90	206.0
154.80	192.0
157.00	128.0
159.00	83.0
172.30	387.0
174.00	39224.0
175.00	3495.0
176.00	40592.0
177.00	2747.0
178.10	101.0
191.00	128.0
193.00	122.0
206.90	101.0
249.00	57.0
249.90	55.0
251.10	94.0
264.80	102.0
265.30	135.0

Instrument :
MSVOA_W
ClientSampleId :
BFB455

281.20	1099.0
281.90	232.0
283.20	256.0

Instrument :
MSVOA_W
ClientSampleId :
BFB455

m/z	Abundance
36.00	383.0
37.00	1757.0
38.10	1824.0
39.10	786.0
40.20	179.0
44.00	407.0
45.00	368.0
47.00	558.0
48.10	250.0
49.00	1755.0
50.10	7656.0
51.10	2519.0
52.10	131.0
55.00	151.0
56.00	693.0
57.00	1190.0
60.00	405.0
61.00	1954.0
62.10	2129.0
63.10	1820.0
64.10	200.0
65.10	192.0
67.10	157.0
68.00	4614.0
69.00	4612.0
70.10	250.0
72.30	206.0
73.00	2105.0
74.00	8030.0
75.10	21408.0
76.00	2055.0
77.10	344.0
78.00	133.0
79.00	1287.0
80.00	472.0
81.00	1432.0
82.00	336.0
85.90	57.0
87.00	1526.0
88.00	1383.0
91.00	248.0
92.00	1335.0
93.00	1931.0
94.00	4944.0
95.00	39792.0
96.10	2782.0
97.00	89.0
103.90	184.0
104.80	87.0
106.00	243.0
111.90	57.0
115.90	265.0
116.90	353.0
117.90	145.0
118.80	287.0
127.80	190.0
128.90	116.0
130.00	158.0
130.90	52.0
133.20	74.0
135.10	58.0
136.70	71.0
141.00	492.0
141.80	82.0
143.00	456.0
145.00	96.0
145.80	77.0
148.00	100.0
155.00	126.0
157.00	114.0
161.00	69.0
171.00	88.0
171.90	231.0
174.00	37592.0
175.00	2960.0
176.00	33608.0
177.00	2046.0
178.10	114.0
207.20	52.0
264.80	51.0
281.20	626.0
282.00	117.0
283.00	66.0

Instrument :
MSVOA_W
ClientSampleId :
BFB455