

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032123\
 Data File : VW025458.D
 Acq On : 21 Mar 2023 11:05
 Operator : SY/MD
 Sample : 01979-17
 Misc : 5.67g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGC8

Quant Time: Mar 22 01:31:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 22 01:30:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1004255	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	904201	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	396381	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	194897	11.672	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	46.680%
7) Chloroethane-d5	2.899	69	192574	16.028	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.120%
11) 1,1-Dichloroethene-d2	4.021	63	420798	13.048	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	52.200%
21) 2-Butanone-d5	7.075	46	242882	59.260	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	118.520%
24) Chloroform-d	7.648	84	628951	21.724	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.880%
26) 1,2-Dichloroethane-d4	8.307	65	382969	24.645	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.600%
32) Benzene-d6	8.270	84	1284813	20.795	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.200%
36) 1,2-Dichloropropane-d6	9.276	67	431858	22.595	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.360%
41) Toluene-d8	10.325	98	1150450	21.120	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.480%
43) trans-1,3-Dichloroprop...	10.575	79	175220	23.022	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.080%
47) 2-Hexanone-d5	10.922	63	171224	62.299	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	124.600%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	368283	26.300	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.200%
66) 1,2-Dichlorobenzene-d4	13.849	152	366103	24.837	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.360%
Target Compounds					Qvalue	
13) Acetone	4.119	43	113162	28.721	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032123\
Data File : VW025458.D
Acq On : 21 Mar 2023 11:05
Operator : SY/MD
Sample : 01979-17
Misc : 5.67g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EYGC8

Quant Time: Mar 22 01:31:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 22 01:30:00 2023
Response via : Initial Calibration

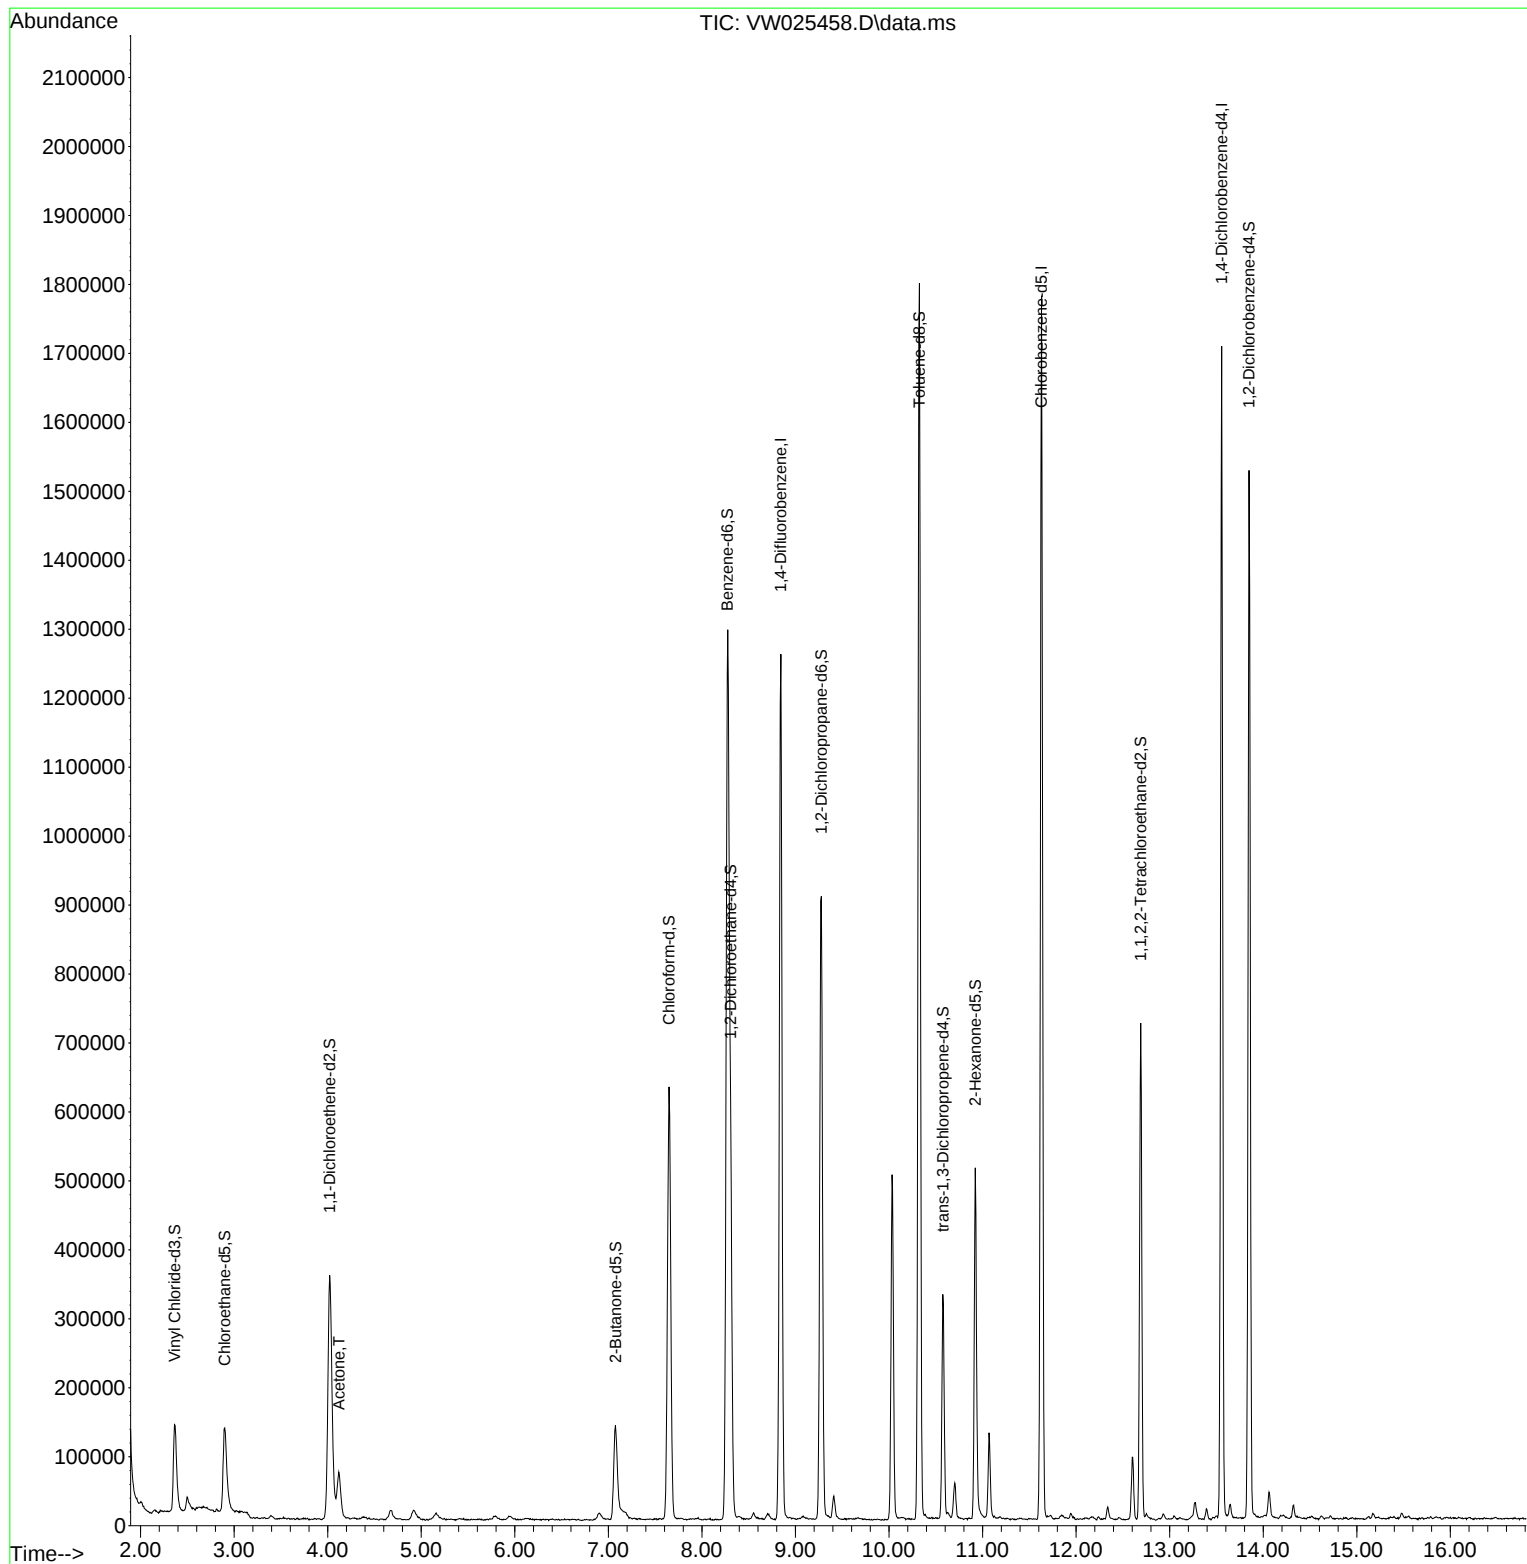

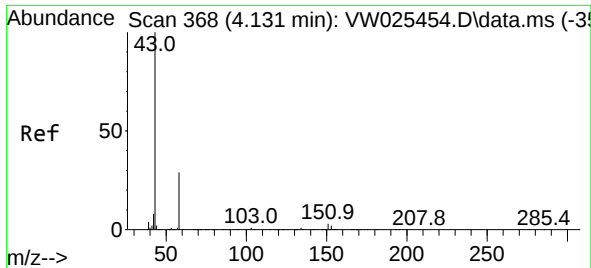

#13
 Acetone
 Concen: 28.721 ug/L
 RT: 4.119 min Scan# 30
 Delta R.T. -0.012 min
 Lab File: VW025458.D
 Acq: 21 Mar 2023 11:05

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGC8

Tgt Ion: 43 Resp: 113162
 Ion Ratio Lower Upper
 43 100
 58 29.7 0.0 60.0

