

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032123\
 Data File : VW025471.D
 Acq On : 21 Mar 2023 16:16
 Operator : SY/MD
 Sample : 01979-11RE
 Misc : 5.93g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB6

Quant Time: Mar 22 01:35:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 22 01:30:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	975062	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	903358	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	438756	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	158666	9.787	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	39.160%
7) Chloroethane-d5	2.899	69	157255	13.480	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	53.920%
11) 1,1-Dichloroethene-d2	4.027	63	344929	11.015	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	44.080%#
21) 2-Butanone-d5	7.075	46	237171	59.599	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	119.200%
24) Chloroform-d	7.648	84	537240	19.112	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	76.440%
26) 1,2-Dichloroethane-d4	8.306	65	335185	22.216	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.880%
32) Benzene-d6	8.270	84	1098354	17.794	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	71.160%
36) 1,2-Dichloropropane-d6	9.270	67	372229	19.493	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	77.960%
41) Toluene-d8	10.318	98	975323	17.921	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	71.680%
43) trans-1,3-Dichloroprop...	10.574	79	152628	20.073	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.280%
47) 2-Hexanone-d5	10.922	63	164176	59.790	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	119.580%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	338880	24.223	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.880%
66) 1,2-Dichlorobenzene-d4	13.848	152	336924	20.650	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	82.600%
Target Compounds					Qvalue	
13) Acetone	4.124	43	46520	12.161	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032123\
Data File : VW025471.D
Acq On : 21 Mar 2023 16:16
Operator : SY/MD
Sample : 01979-11RE
Misc : 5.93g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EYGB6

Quant Time: Mar 22 01:35:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 22 01:30:00 2023
Response via : Initial Calibration

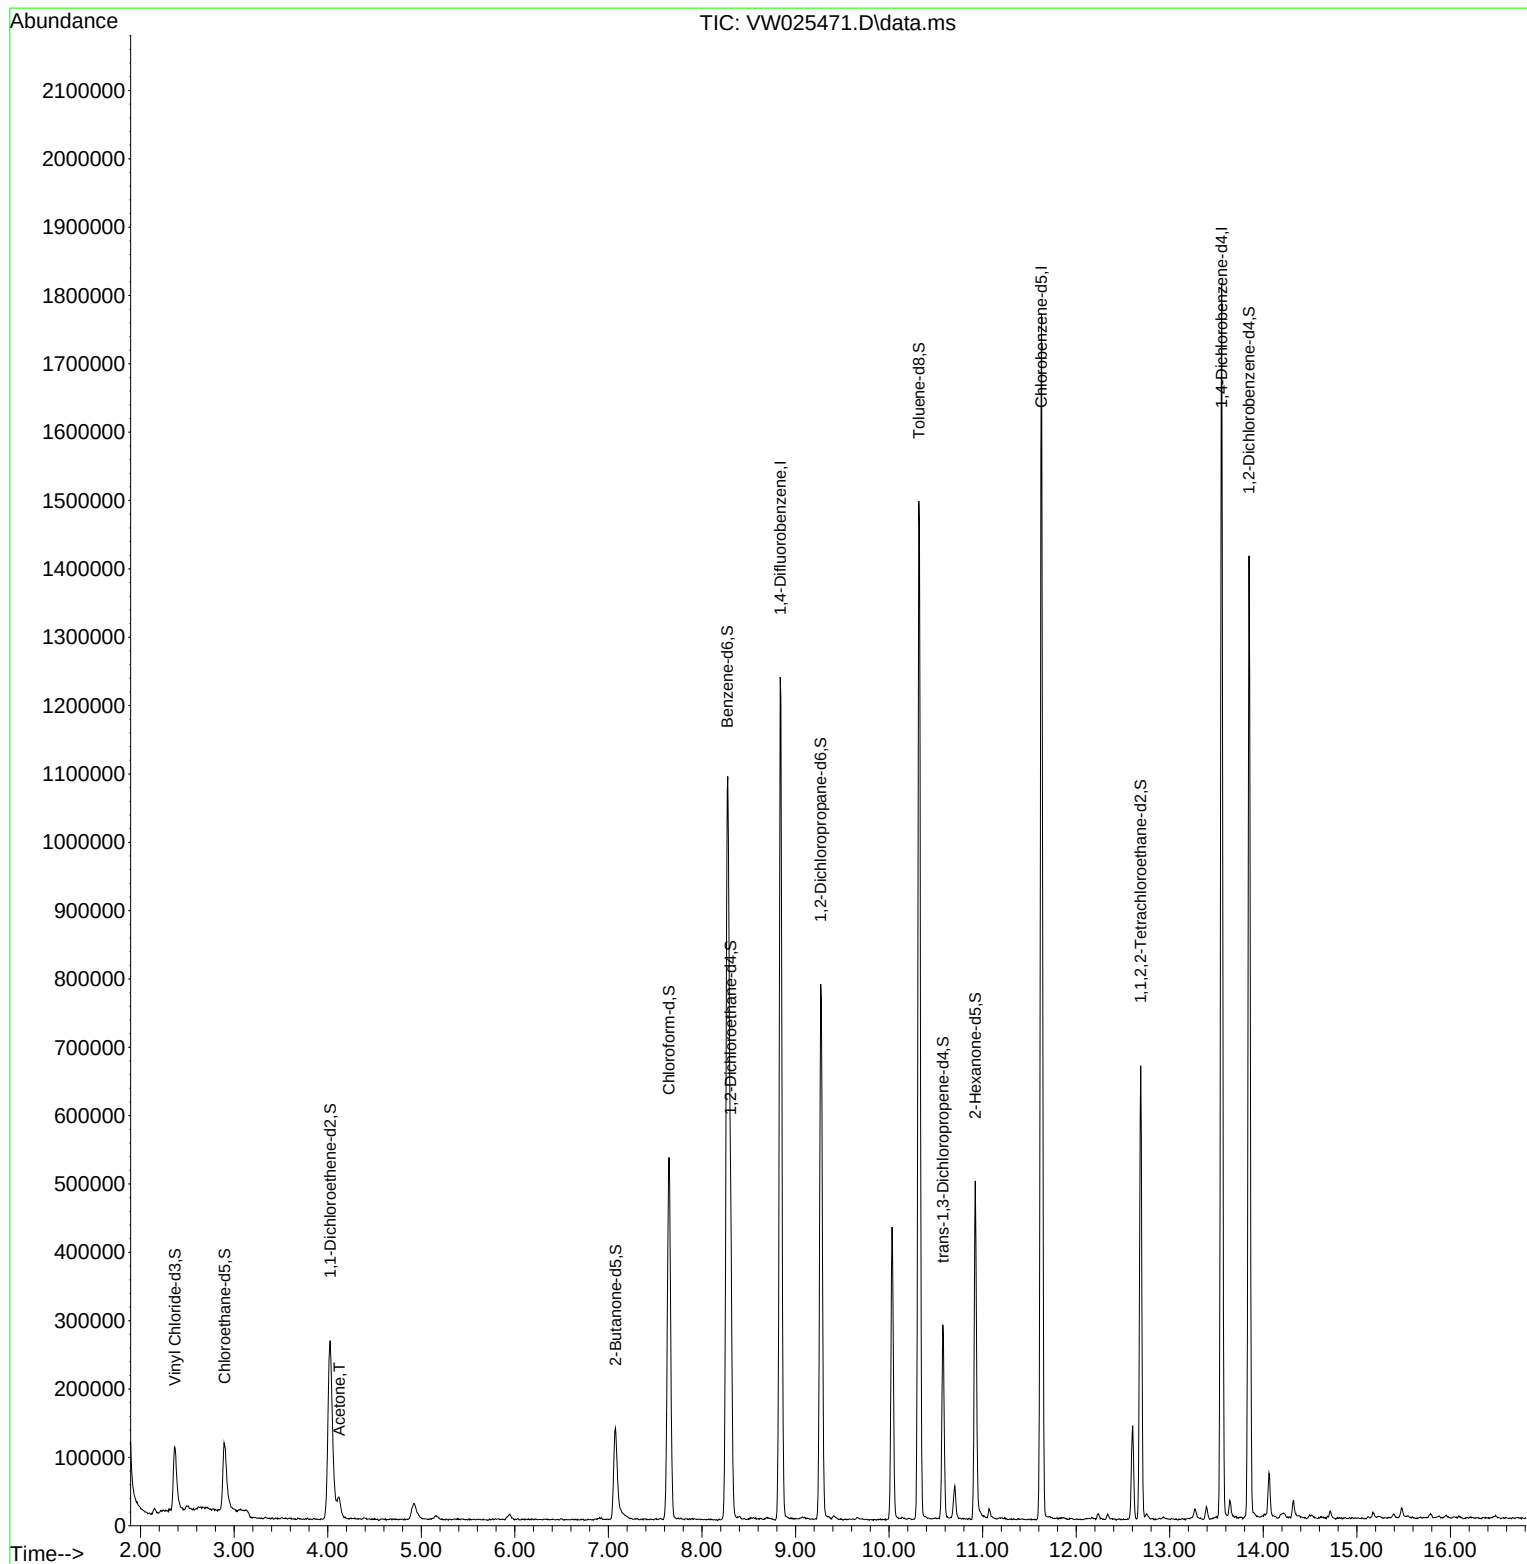

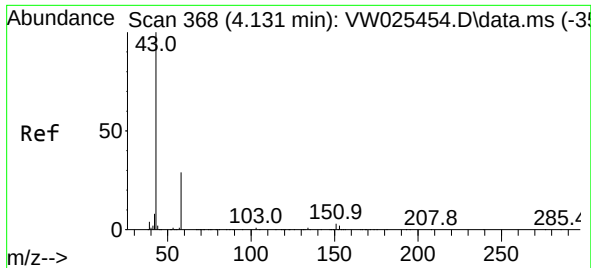

#13
 Acetone
 Concen: 12.161 ug/L
 RT: 4.124 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW025471.D
 Acq: 21 Mar 2023 16:16

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB6

Tgt Ion: 43 Resp: 46520
 Ion Ratio Lower Upper
 43 100
 58 30.4 0.0 60.0

