




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032123\
 Data File : VW025457.D
 Acq On : 21 Mar 2023 10:41
 Operator : SY/MD
 Sample : 01979-03
 Misc : 9.35g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB9

Manual IntegrationsAPPROVED

Quant Time: Mar 22 01:30:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 22 01:30:00 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/22/2023
 Supervised By :Mahesh Dadoda 03/22/2023

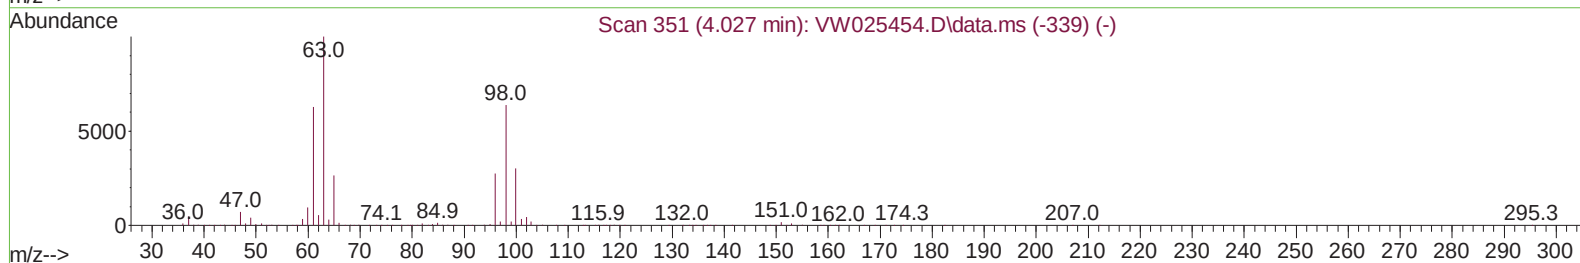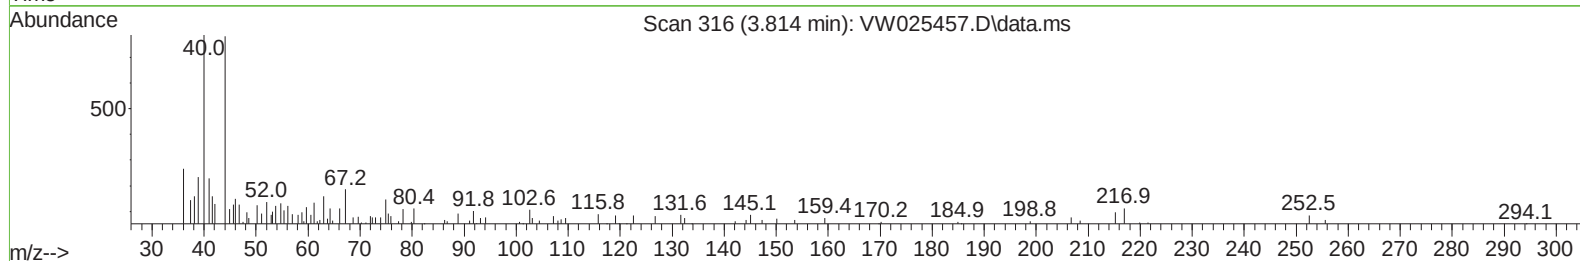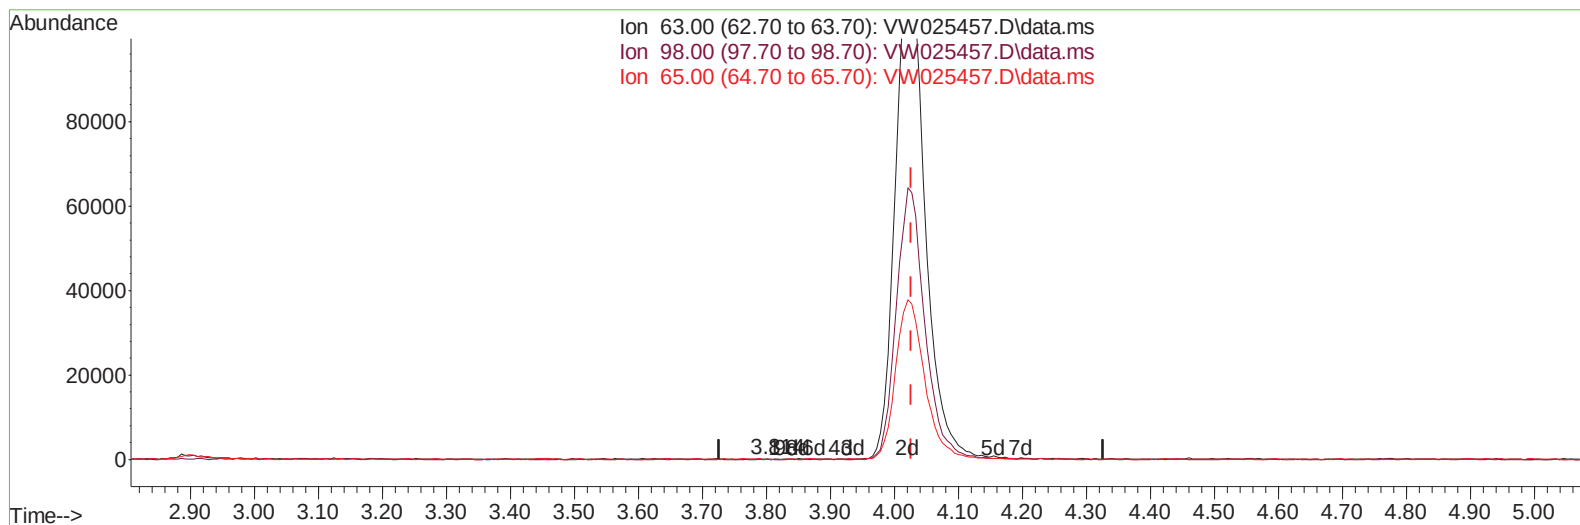

TIC: VW025457.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.814min (-0.214) 0.00 ug/L

response 87

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.90	71.26
65.00	23.70	26.44
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032123\
 Data File : VW025457.D
 Acq On : 21 Mar 2023 10:41
 Operator : SY/MD
 Sample : 01979-03
 Misc : 9.35g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB9

Manual IntegrationsAPPROVED

Quant Time: Mar 22 01:30:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 22 01:30:00 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/22/2023
 Supervised By :Mahesh Dadoda 03/22/2023

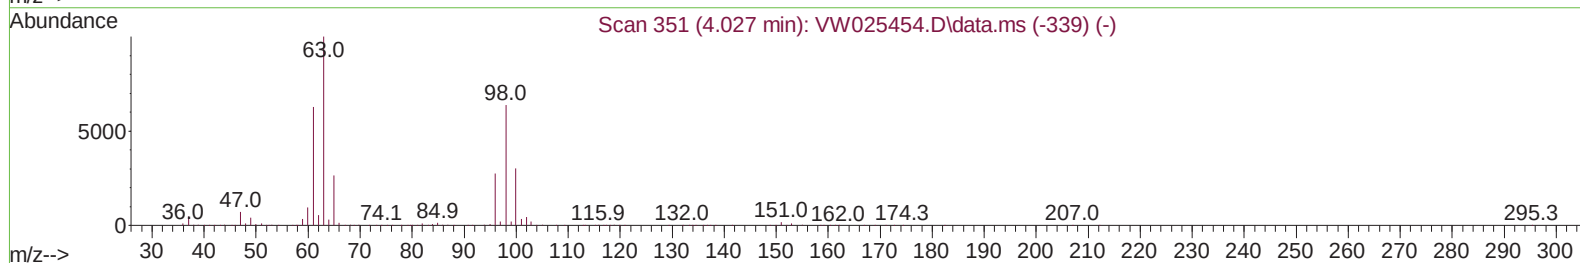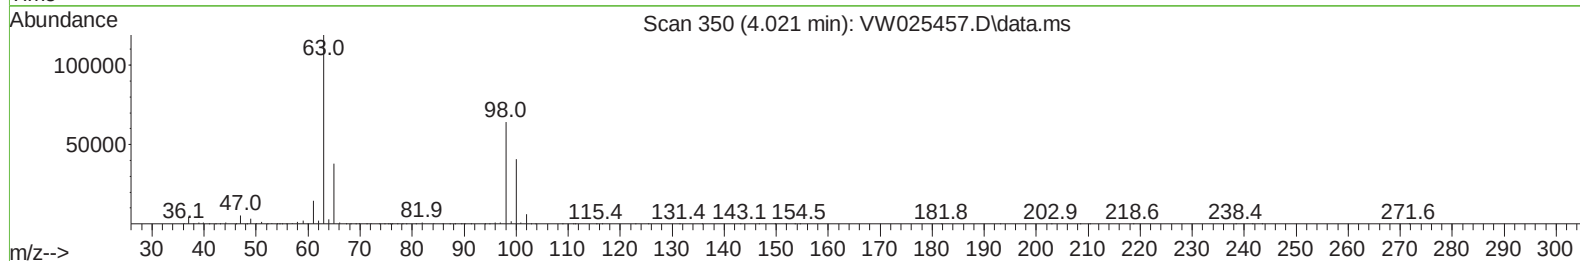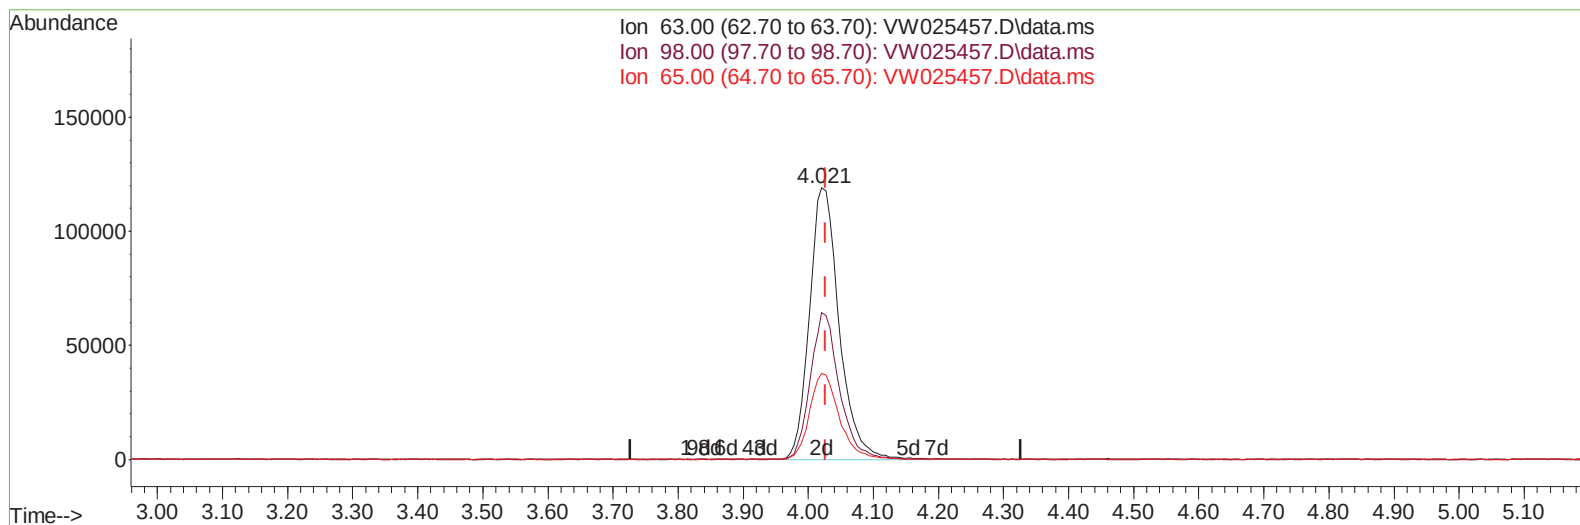

TIC: VW025457.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.021min (-0.006) 12.93 ug/L m

response 377944

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.90	0.02#
65.00	23.70	0.01#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032123\
 Data File : VW025457.D
 Acq On : 21 Mar 2023 10:41
 Operator : SY/MD
 Sample : 01979-03
 Misc : 9.35g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/22/2023
 Supervised By :Mahesh Dadoda 03/22/2023

Quant Time: Mar 22 01:30:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 22 01:30:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	910493	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	812264	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	345511	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	174777	11.545	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	46.200%	
7) Chloroethane-d5	2.899	69	172654	15.850	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	63.400%	
11) 1,1-Dichloroethene-d2	4.021	63	377944m	12.926	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	51.720%	
21) 2-Butanone-d5	7.075	46	252125	67.850	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	135.700%#	
24) Chloroform-d	7.648	84	565918	21.560	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	86.240%	
26) 1,2-Dichloroethane-d4	8.307	65	362884	25.758	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	103.040%	
32) Benzene-d6	8.276	84	1173117	21.137	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	84.560%	
36) 1,2-Dichloropropane-d6	9.276	67	394737	22.990	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	91.960%	
41) Toluene-d8	10.325	98	1034471	21.140	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	84.560%	
43) trans-1,3-Dichloroprop...	10.575	79	163701	23.943	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	95.760%	
47) 2-Hexanone-d5	10.922	63	172486	69.861	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	139.720%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	359808	28.604	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	114.400%	
66) 1,2-Dichlorobenzene-d4	13.848	152	304944	23.733	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	94.920%	
Target Compounds					Qvalue	
13) Acetone	4.124	43	107072	29.974	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032123\
Data File : VW025457.D
Acq On : 21 Mar 2023 10:41
Operator : SY/MD
Sample : 01979-03
Misc : 9.35g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EYGB9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/22/2023
Supervised By :Mahesh Dadoda 03/22/2023

Quant Time: Mar 22 01:30:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 22 01:30:00 2023
Response via : Initial Calibration

