




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032123\
 Data File : VW025464.D
 Acq On : 21 Mar 2023 13:28
 Operator : SY/MD
 Sample : 01979-11
 Misc : 7.18g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB6

Manual IntegrationsAPPROVED

Quant Time: Mar 22 01:33:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 22 01:30:00 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/22/2023
 Supervised By :Mahesh Dadoda 03/22/2023

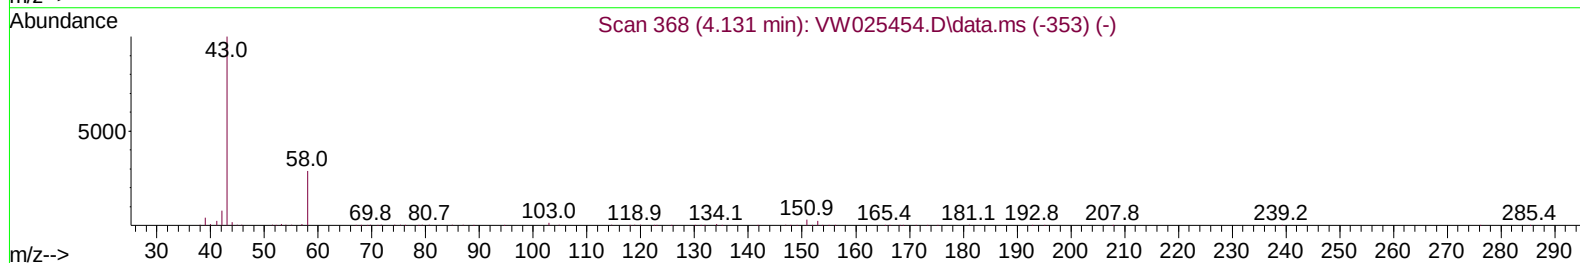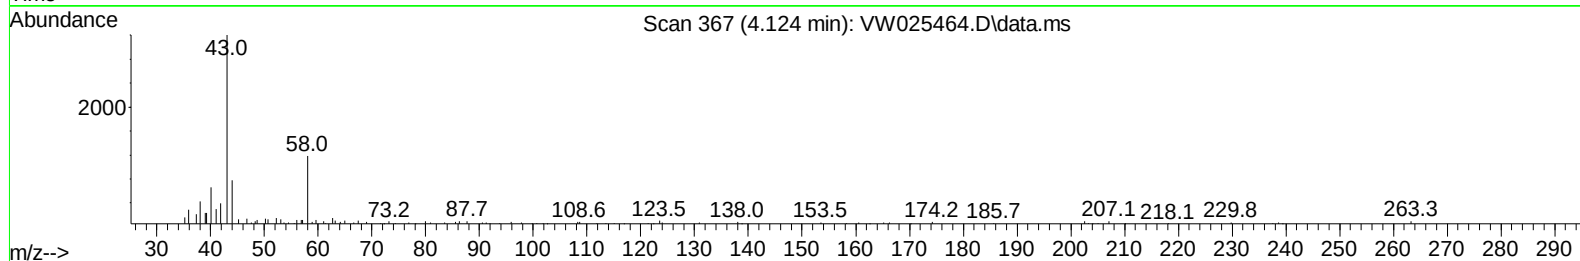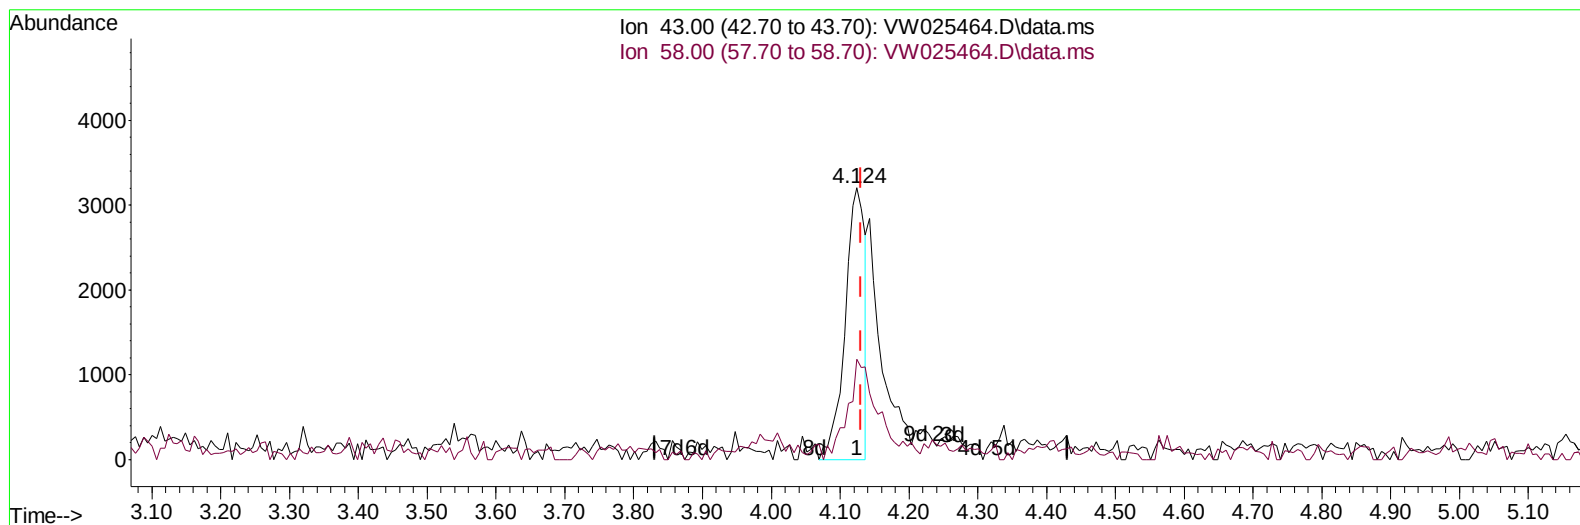

TIC: VW025464.D\data.ms

(13) Acetone (T)

4.124min (-0.006) 10.43 ug/L

response 6430

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.00	53.84
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032123\
 Data File : VW025464.D
 Acq On : 21 Mar 2023 13:28
 Operator : SY/MD
 Sample : 01979-11
 Misc : 7.18g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB6

Manual IntegrationsAPPROVED

Quant Time: Mar 22 01:33:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 22 01:30:00 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/22/2023
 Supervised By :Mahesh Dadoda 03/22/2023

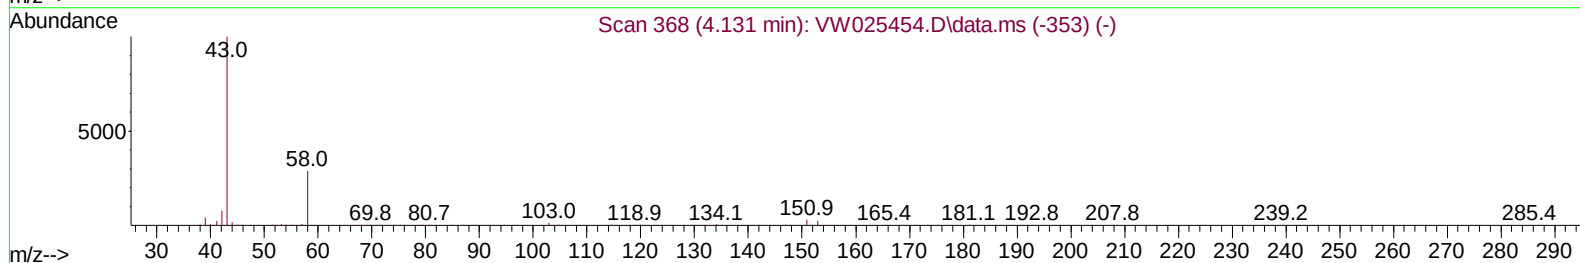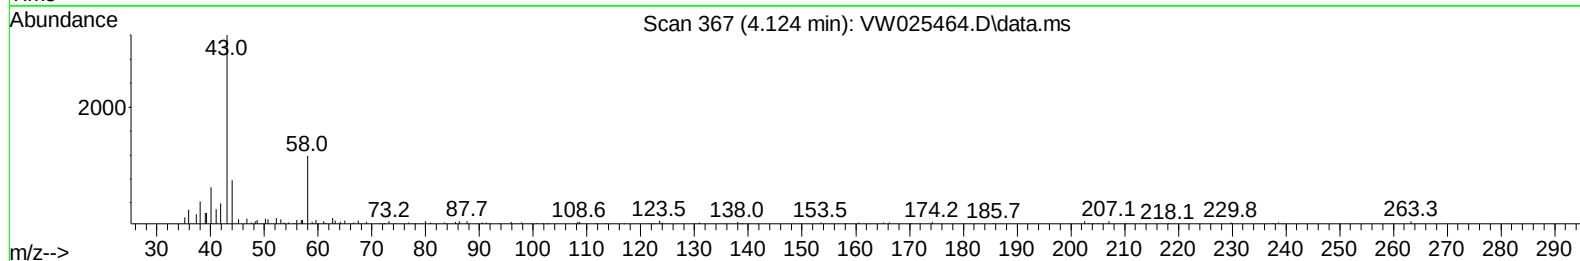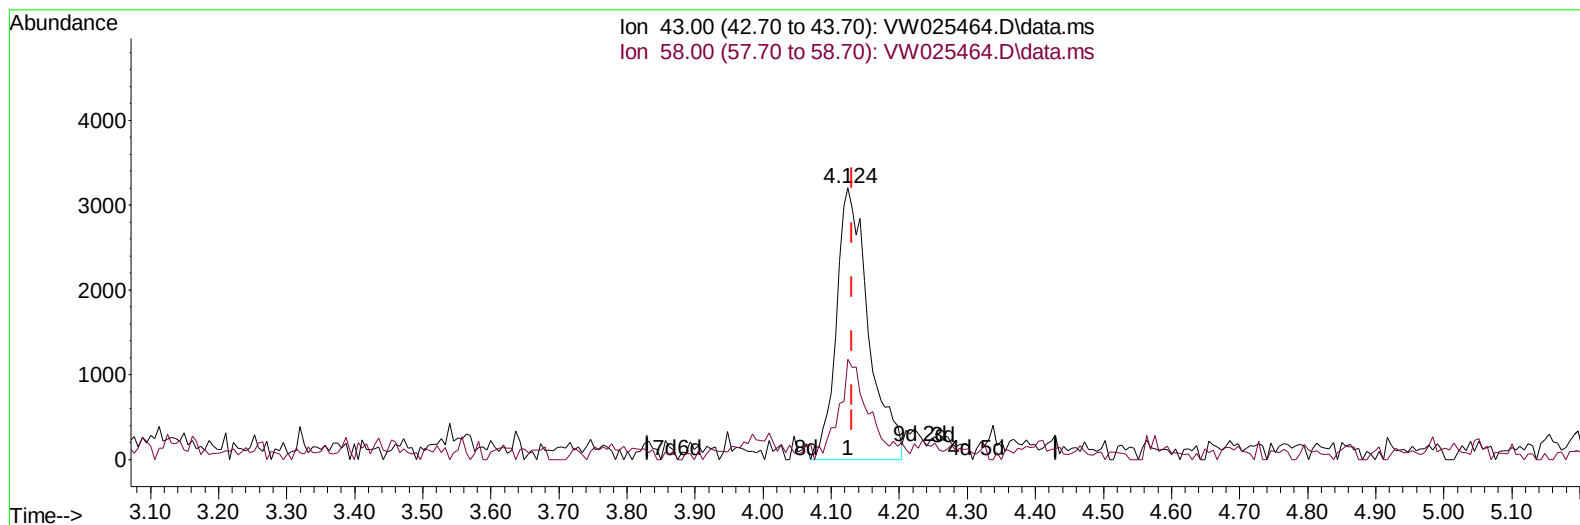

TIC: VW025464.D\data.ms

(13) Acetone (T)

4.124min (-0.006) 17.13 ug/L m

response 10557

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.00	32.79
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032123\
 Data File : VW025464.D
 Acq On : 21 Mar 2023 13:28
 Operator : SY/MD
 Sample : 01979-11
 Misc : 7.18g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB6

Manual IntegrationsAPPROVED

Quant Time: Mar 22 01:33:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 22 01:30:00 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/22/2023
 Supervised By :Mahesh Dadoda 03/22/2023

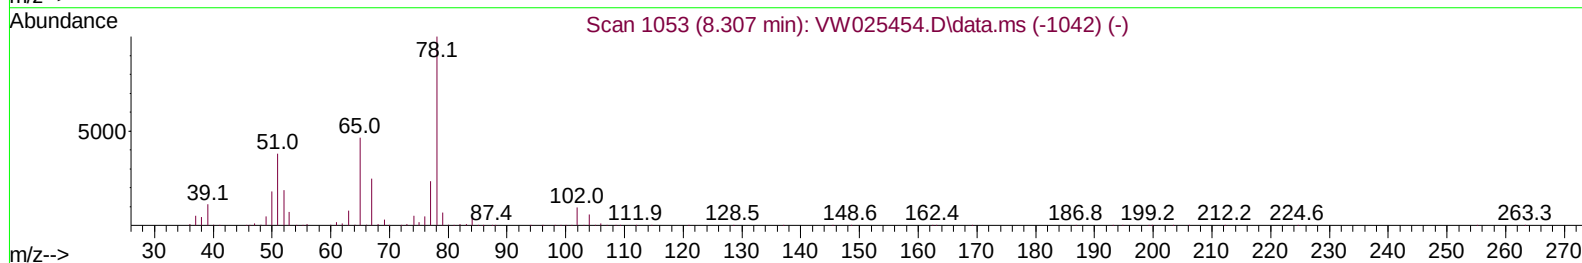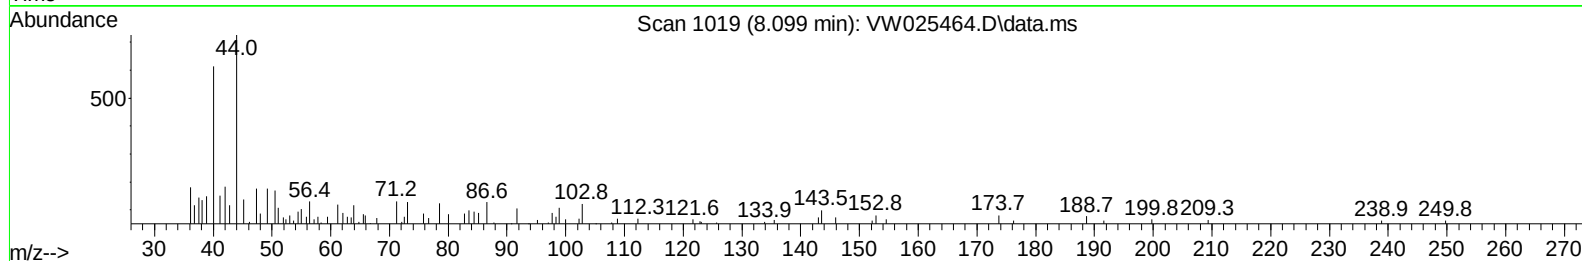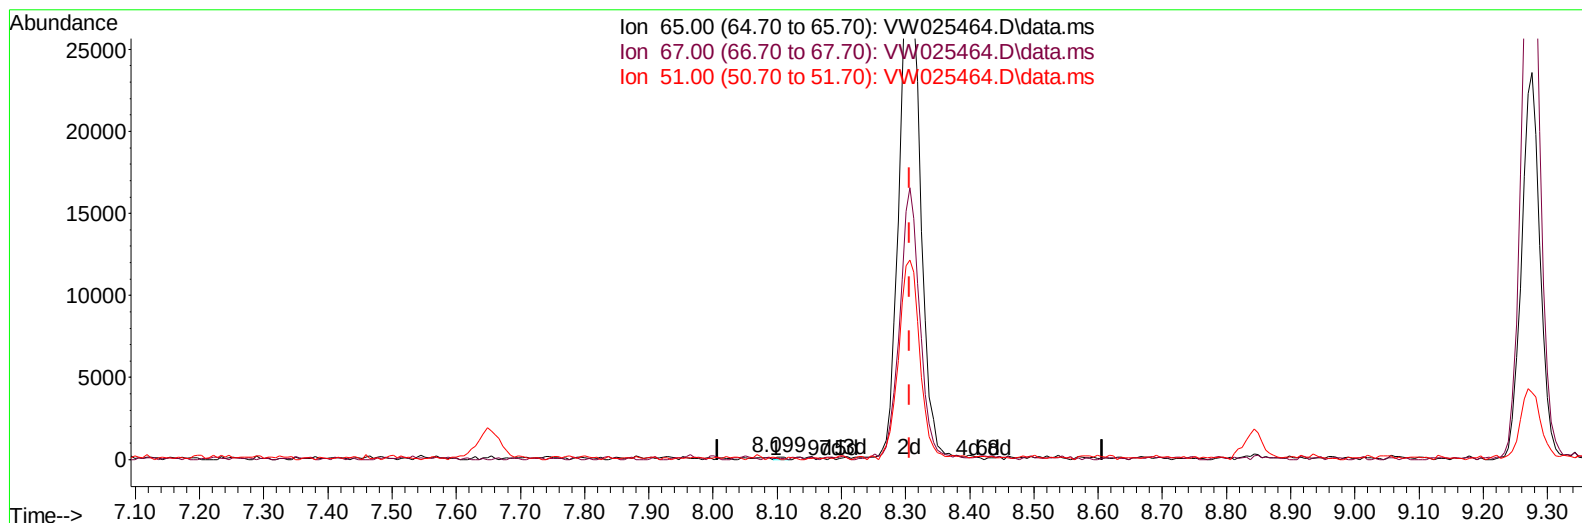

TIC: VW025464.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.099min (-0.207) 0.06 ug/L

response 144

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.30	45.83
51.00	111.10	88.89
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032123\
Data File : VW025464.D
Acq On : 21 Mar 2023 13:28
Operator : SY/MD
Sample : 01979-11
Misc : 7.18g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EYGB6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/22/2023
Supervised By :Mahesh Dadoda 03/22/2023

Quant Time: Mar 22 01:33:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 22 01:30:00 2023
Response via : Initial Calibration

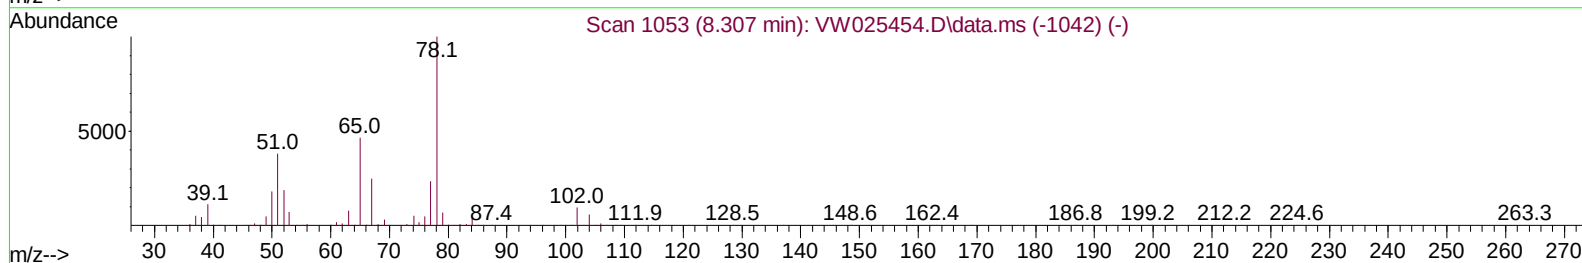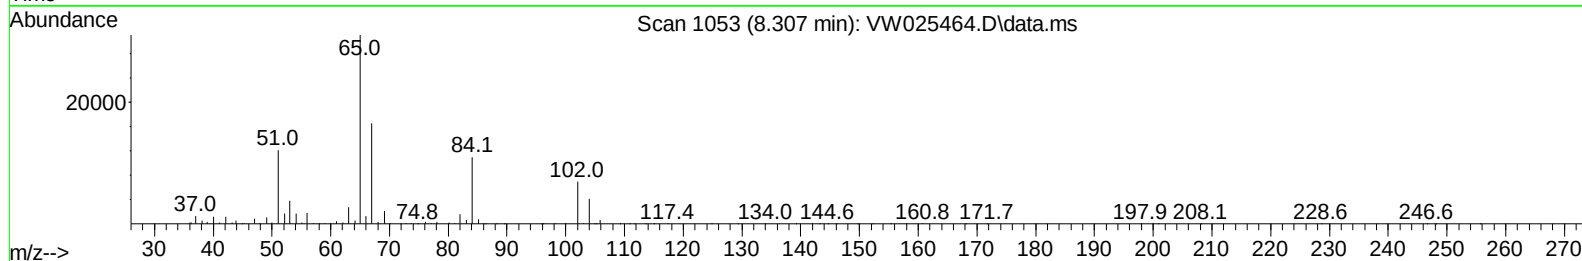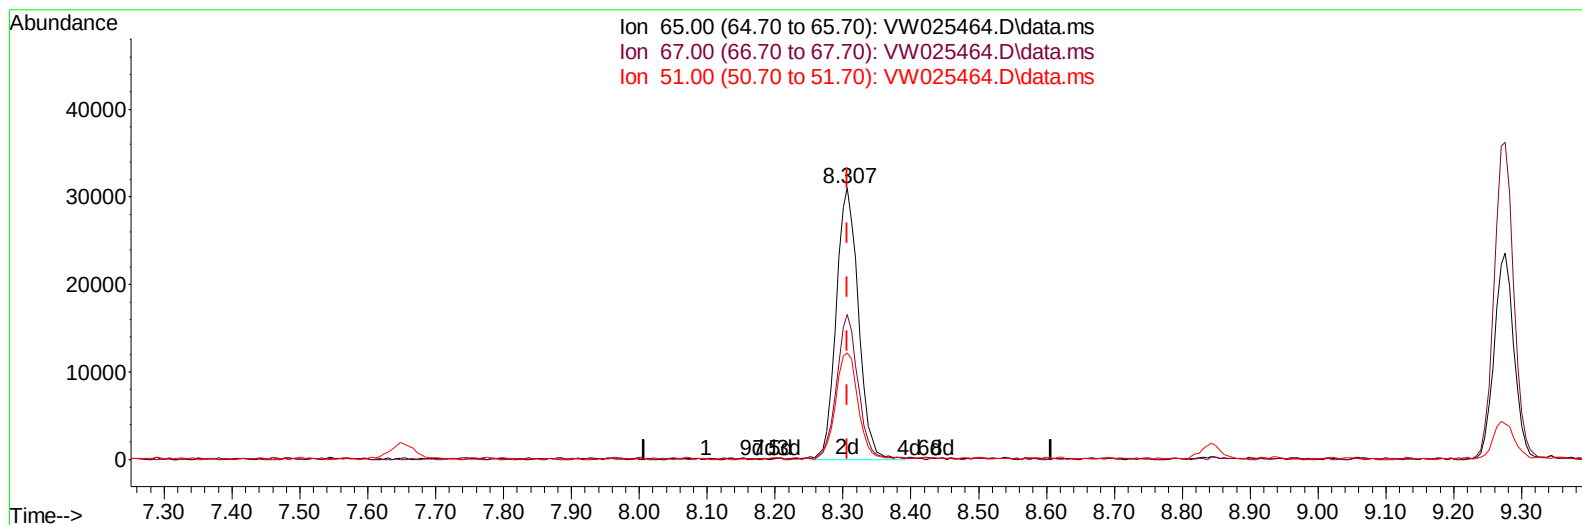

TIC: VW025464.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 28.99 ug/L m

response 70461

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.30	0.09#
51.00	111.10	0.18#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032123\
 Data File : VW025464.D
 Acq On : 21 Mar 2023 13:28
 Operator : SY/MD
 Sample : 01979-11
 Misc : 7.18g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB6

Manual IntegrationsAPPROVED

Quant Time: Mar 22 01:33:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 22 01:30:00 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/22/2023
 Supervised By :Mahesh Dadoda 03/22/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		157079	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		150487	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		65334	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.356	65		32716	12.527	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	50.120%	
7) Chloroethane-d5	2.887	69		34980	18.614	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.440%	
11) 1,1-Dichloroethene-d2	4.021	63		71286	14.132	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.520%	
21) 2-Butanone-d5	7.075	46		43016	67.100	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	134.200%	
24) Chloroform-d	7.648	84		105397	23.275	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.080%	
26) 1,2-Dichloroethane-d4	8.307	65		70461m	28.990	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	115.960%	
32) Benzene-d6	8.276	84		212059	20.623	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.480%	
36) 1,2-Dichloropropane-d6	9.276	67		73134	22.990	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.960%	
41) Toluene-d8	10.324	98		181169	19.983	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.920%	
43) trans-1,3-Dichloroprop...	10.581	79		28314	22.353	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.400%	
47) 2-Hexanone-d5	10.922	63		24869	54.367	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.740%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		71595	30.721	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	122.880%#	
66) 1,2-Dichlorobenzene-d4	13.848	152		63259	26.037	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	104.160%	
Target Compounds							
13) Acetone	4.124	43		10557m	17.130	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032123\
Data File : VW025464.D
Acq On : 21 Mar 2023 13:28
Operator : SY/MD
Sample : 01979-11
Misc : 7.18g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EYGB6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/22/2023
Supervised By :Mahesh Dadoda 03/22/2023

Quant Time: Mar 22 01:33:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 22 01:30:00 2023
Response via : Initial Calibration

