

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032123\
 Data File : VW025457.D
 Acq On : 21 Mar 2023 10:41
 Operator : SY/MD
 Sample : 01979-03
 Misc : 9.35g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB9

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/22/2023
 Supervised By :Mahesh Dadoda 03/22/2023

Quant Time: Mar 22 01:30:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 22 01:30:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	910493	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	812264	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	345511	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	174777	11.545	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	46.200%		
7) Chloroethane-d5	2.899	69	172654	15.850	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	63.400%		
11) 1,1-Dichloroethene-d2	4.021	63	377944m	12.926	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	51.720%		
21) 2-Butanone-d5	7.075	46	252125	67.850	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	135.700%#		
24) Chloroform-d	7.648	84	565918	21.560	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	86.240%		
26) 1,2-Dichloroethane-d4	8.307	65	362884	25.758	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	103.040%		
32) Benzene-d6	8.276	84	1173117	21.137	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	84.560%		
36) 1,2-Dichloropropane-d6	9.276	67	394737	22.990	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	91.960%		
41) Toluene-d8	10.325	98	1034471	21.140	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	84.560%		
43) trans-1,3-Dichloroprop...	10.575	79	163701	23.943	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	95.760%		
47) 2-Hexanone-d5	10.922	63	172486	69.861	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	139.720%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	359808	28.604	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	114.400%		
66) 1,2-Dichlorobenzene-d4	13.848	152	304944	23.733	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	94.920%		
Target Compounds					Qvalue	
13) Acetone	4.124	43	107072	29.974	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032123\
Data File : VW025457.D
Acq On : 21 Mar 2023 10:41
Operator : SY/MD
Sample : 01979-03
Misc : 9.35g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EYGB9

Quant Time: Mar 22 01:30:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 22 01:30:00 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 03/22/2023
Supervised By :Mahesh Dadoda 03/22/2023

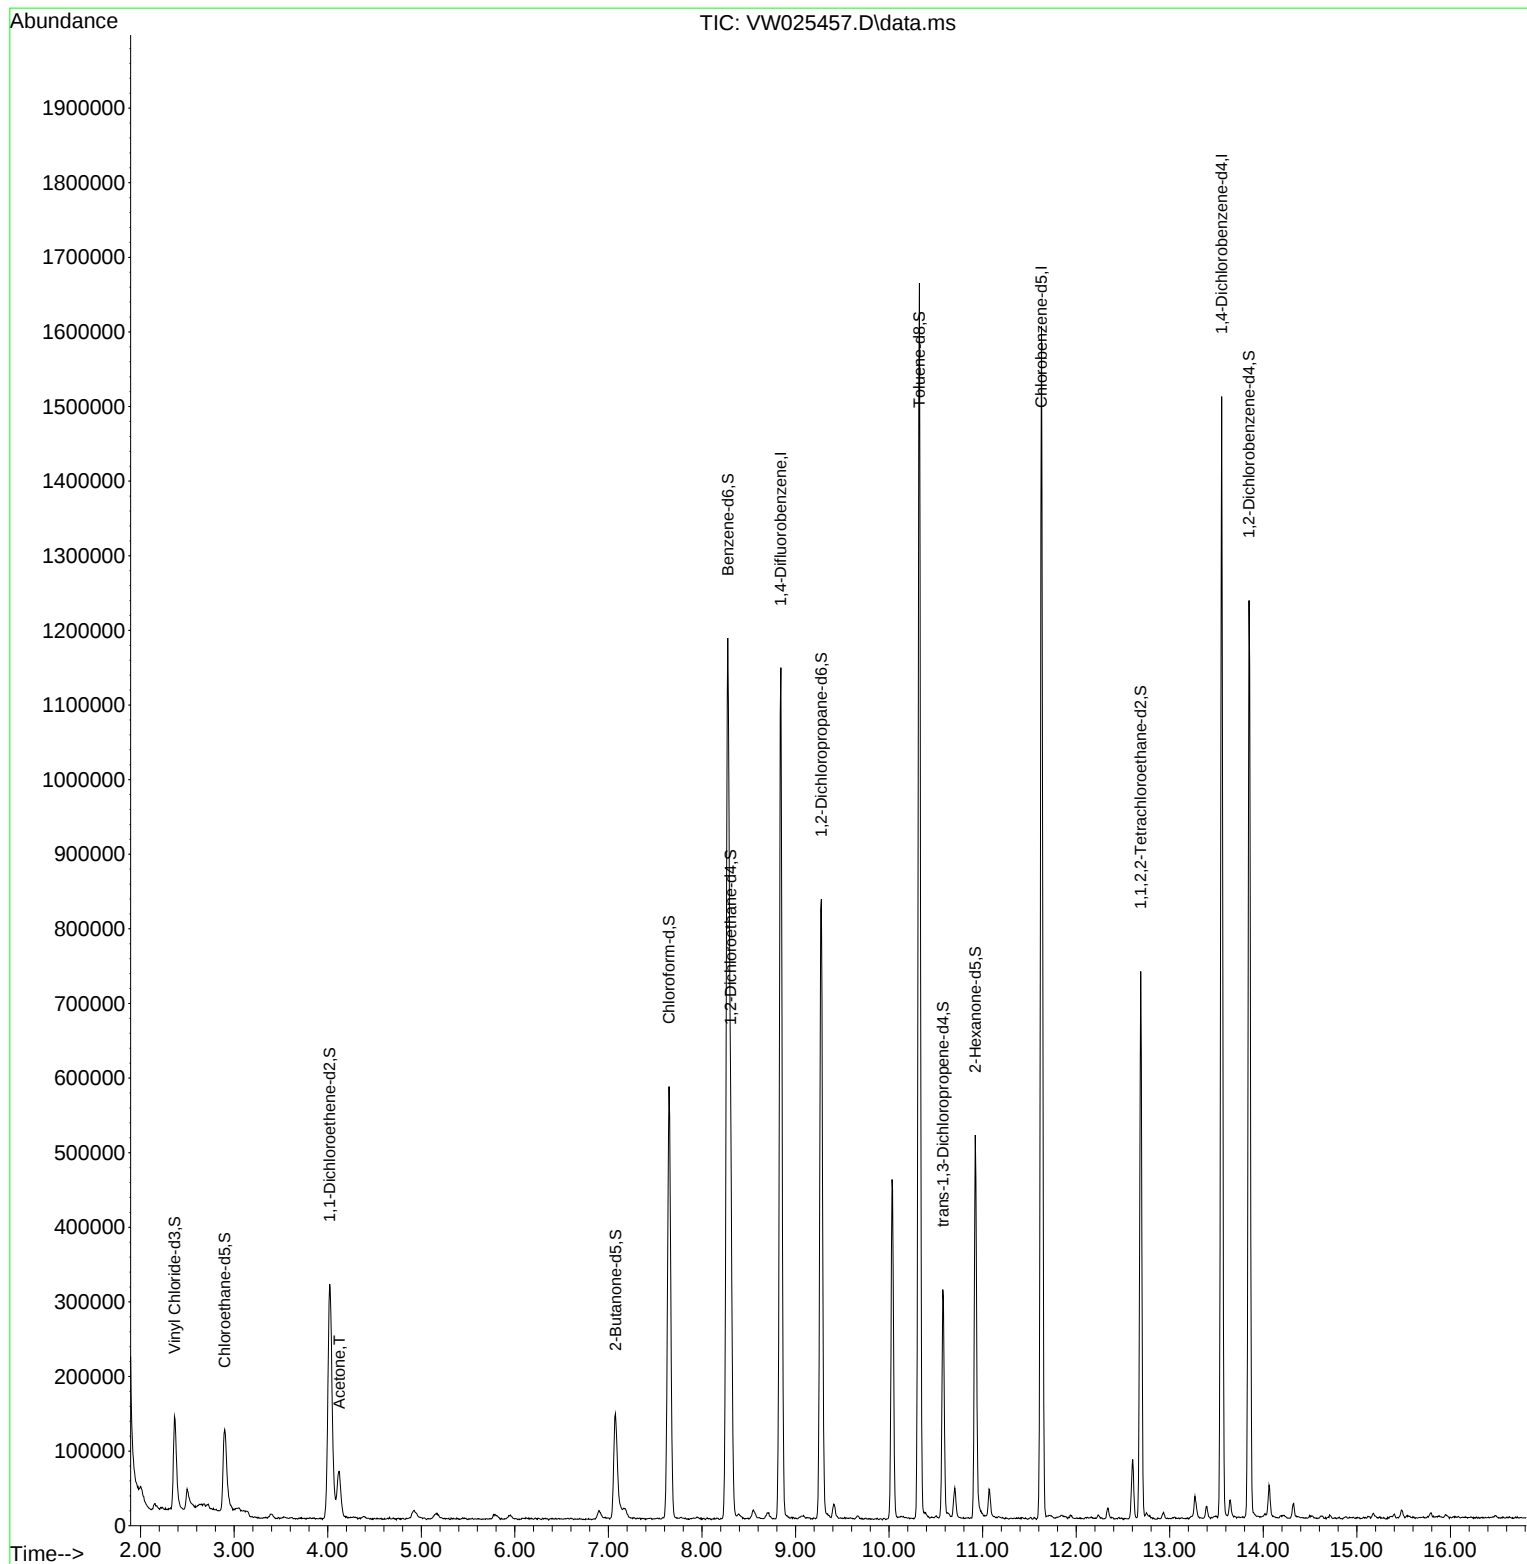

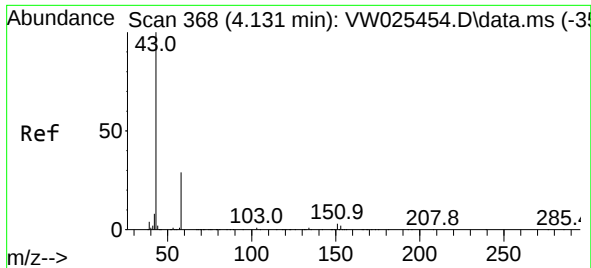

#13
 Acetone
 Concen: 29.974 ug/L
 RT: 4.124 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW025457.D
 Acq: 21 Mar 2023 10:41

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB9

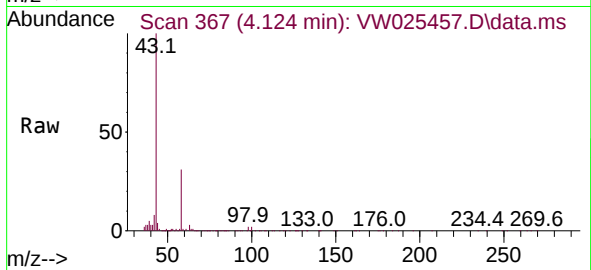

Tgt Ion: 43 Resp: 107072
 Ion Ratio Lower Upper
 43 100
 58 30.6 0.0 60.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/22/2023
 Supervised By :Mahesh Dadoda 03/22/2023

