

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032123\
 Data File : VW025464.D
 Acq On : 21 Mar 2023 13:28
 Operator : SY/MD
 Sample : 01979-11
 Misc : 7.18g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB6

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/22/2023
 Supervised By :Mahesh Dadoda 03/22/2023

Quant Time: Mar 22 01:33:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 22 01:30:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	157079	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	150487	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	65334	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.356	65	32716	12.527	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	50.120%
7) Chloroethane-d5	2.887	69	34980	18.614	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.440%
11) 1,1-Dichloroethene-d2	4.021	63	71286	14.132	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.520%
21) 2-Butanone-d5	7.075	46	43016	67.100	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	134.200%
24) Chloroform-d	7.648	84	105397	23.275	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.080%
26) 1,2-Dichloroethane-d4	8.307	65	70461m	28.990	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	115.960%
32) Benzene-d6	8.276	84	212059	20.623	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.480%
36) 1,2-Dichloropropane-d6	9.276	67	73134	22.990	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.960%
41) Toluene-d8	10.324	98	181169	19.983	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.920%
43) trans-1,3-Dichloroprop...	10.581	79	28314	22.353	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.400%
47) 2-Hexanone-d5	10.922	63	24869	54.367	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.740%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	71595	30.721	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	122.880%#
66) 1,2-Dichlorobenzene-d4	13.848	152	63259	26.037	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	104.160%
Target Compounds					Qvalue	
13) Acetone	4.124	43	10557m	17.130	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032123\
Data File : VW025464.D
Acq On : 21 Mar 2023 13:28
Operator : SY/MD
Sample : 01979-11
Misc : 7.18g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EYGB6

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 03/22/2023
Supervised By : Mahesh Dadoda 03/22/2023


Quant Time: Mar 22 01:33:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 22 01:30:00 2023
Response via : Initial Calibration

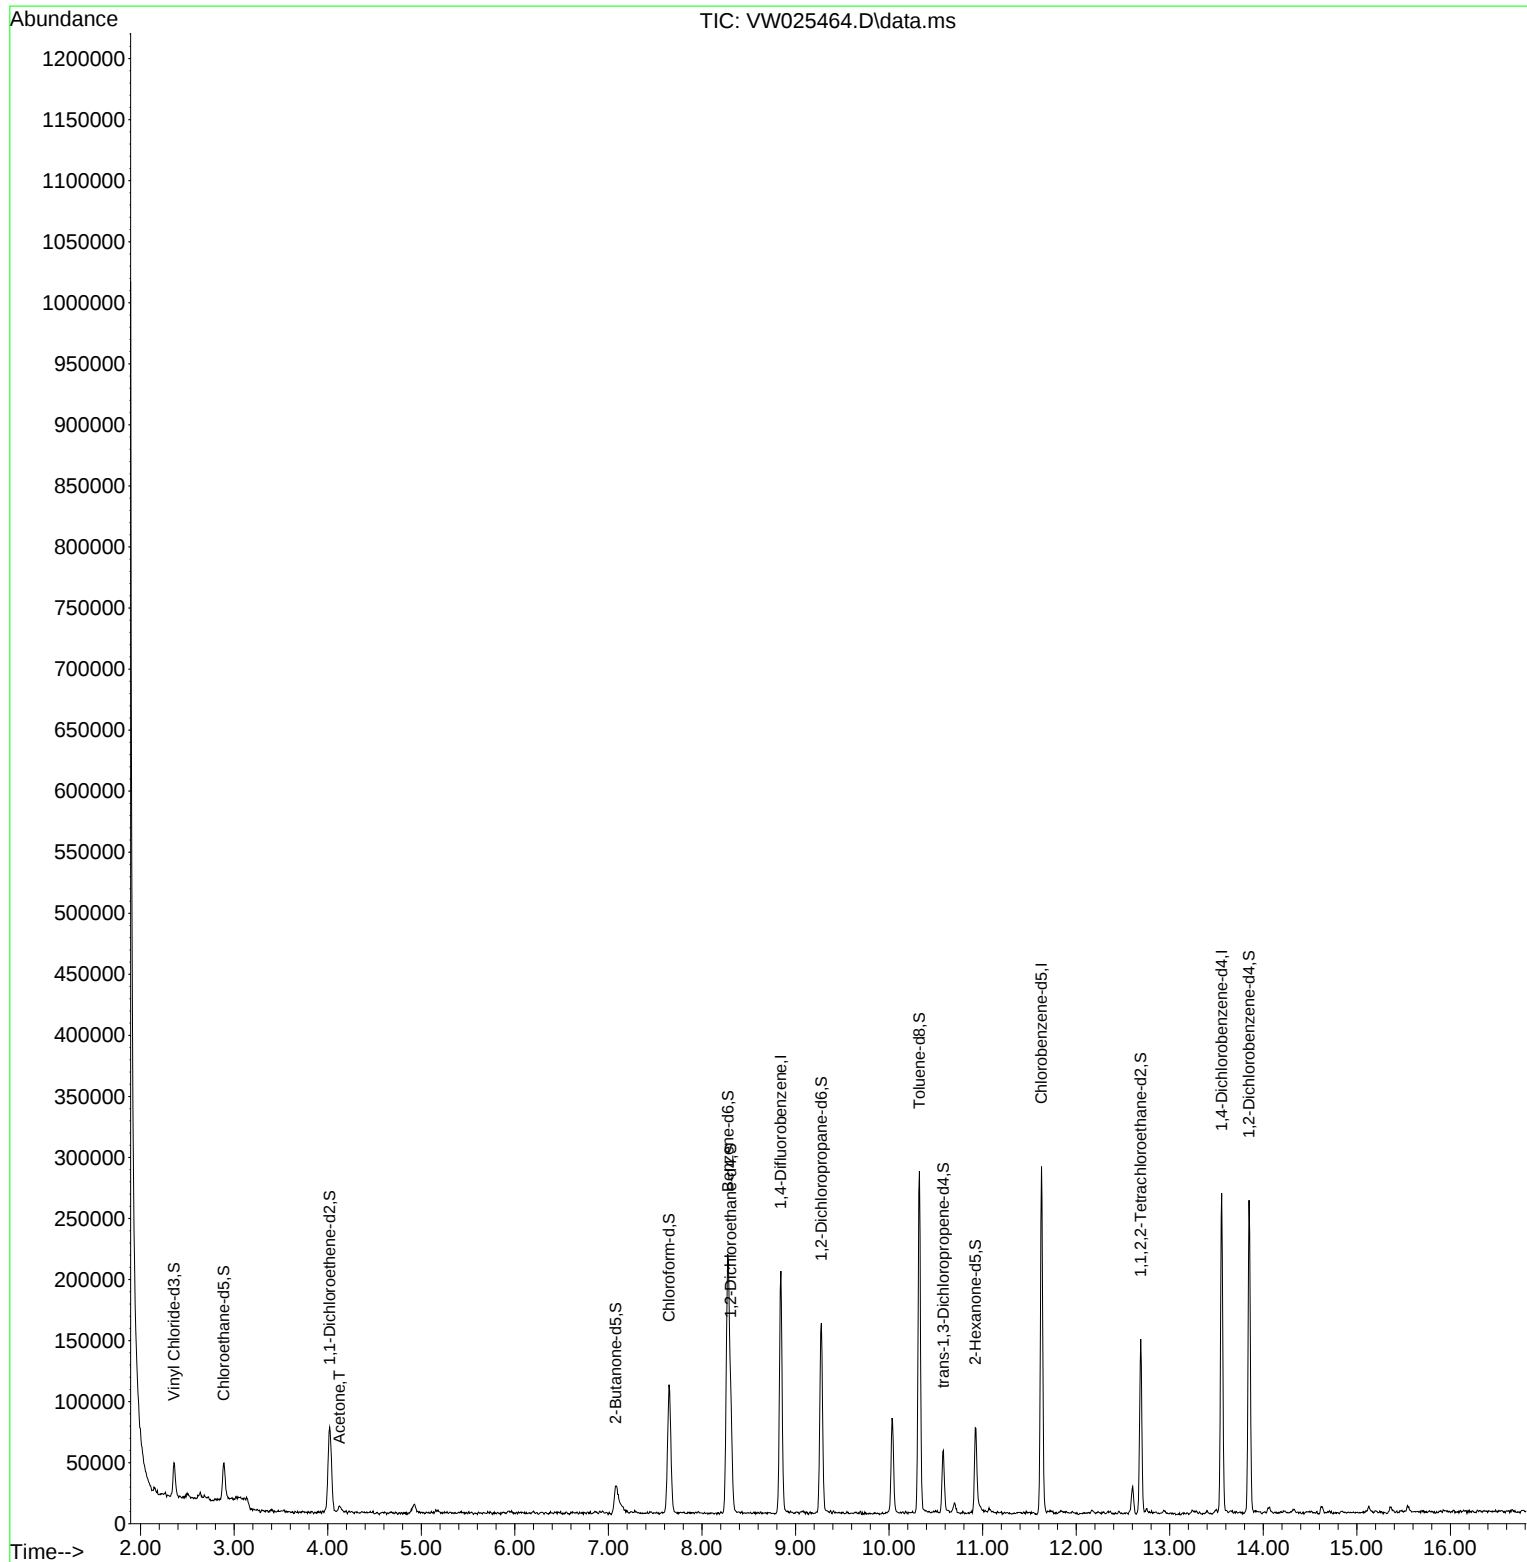

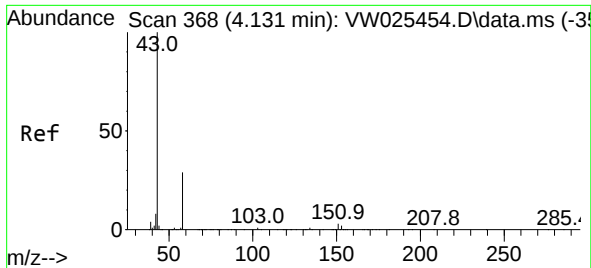

#13
Acetone
Concen: 17.130 ug/L m
RT: 4.124 min Scan# 30
Delta R.T. -0.006 min
Lab File: VW025464.D
Acq: 21 Mar 2023 13:28

Instrument :
MSVOA_W
ClientSampleId :
EYGB6

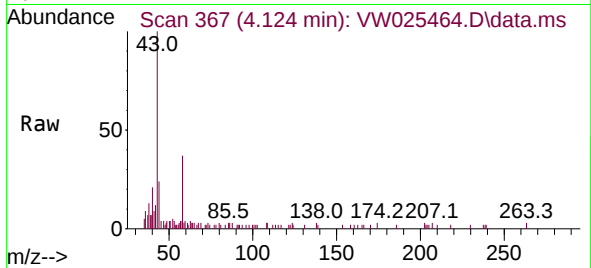

Tgt Ion: 43 Resp: 1055
Ion Ratio Lower Upper
43 100
58 32.8 0.0 60.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 03/22/2023
Supervised By :Mahesh Dadoda 03/22/2023

