

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032123\
 Data File : VW025468.D
 Acq On : 21 Mar 2023 15:04
 Operator : SY/MD
 Sample : 01979-15
 Misc : 6.38g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGC1

Quant Time: Mar 22 01:34:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 22 01:30:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	953730	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	889556	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	409315	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	166558	10.503	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	42.000%
7) Chloroethane-d5	2.899	69	169288	14.836	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.360%
11) 1,1-Dichloroethene-d2	4.027	63	362367	11.831	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	47.320%
21) 2-Butanone-d5	7.075	46	270753	69.559	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	139.120%#
24) Chloroform-d	7.648	84	555357	20.199	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.800%
26) 1,2-Dichloroethane-d4	8.301	65	361238	24.478	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.920%
32) Benzene-d6	8.276	84	1142298	18.793	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	75.160%
36) 1,2-Dichloropropane-d6	9.270	67	395289	21.022	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.080%
41) Toluene-d8	10.319	98	1021249	19.056	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.240%
43) trans-1,3-Dichloroprop...	10.575	79	161417	21.558	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.240%
47) 2-Hexanone-d5	10.922	63	189098	69.935	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	139.860%#
56) 1,1,2,2-Tetrachloroeth...	12.690	84	388760	28.220	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	112.880%
66) 1,2-Dichlorobenzene-d4	13.848	152	344792	22.652	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.600%
Target Compounds					Qvalue	
13) Acetone	4.118	43	44526	11.900	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032123\
Data File : VW025468.D
Acq On : 21 Mar 2023 15:04
Operator : SY/MD
Sample : 01979-15
Misc : 6.38g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EYGC1

Quant Time: Mar 22 01:34:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 22 01:30:00 2023
Response via : Initial Calibration

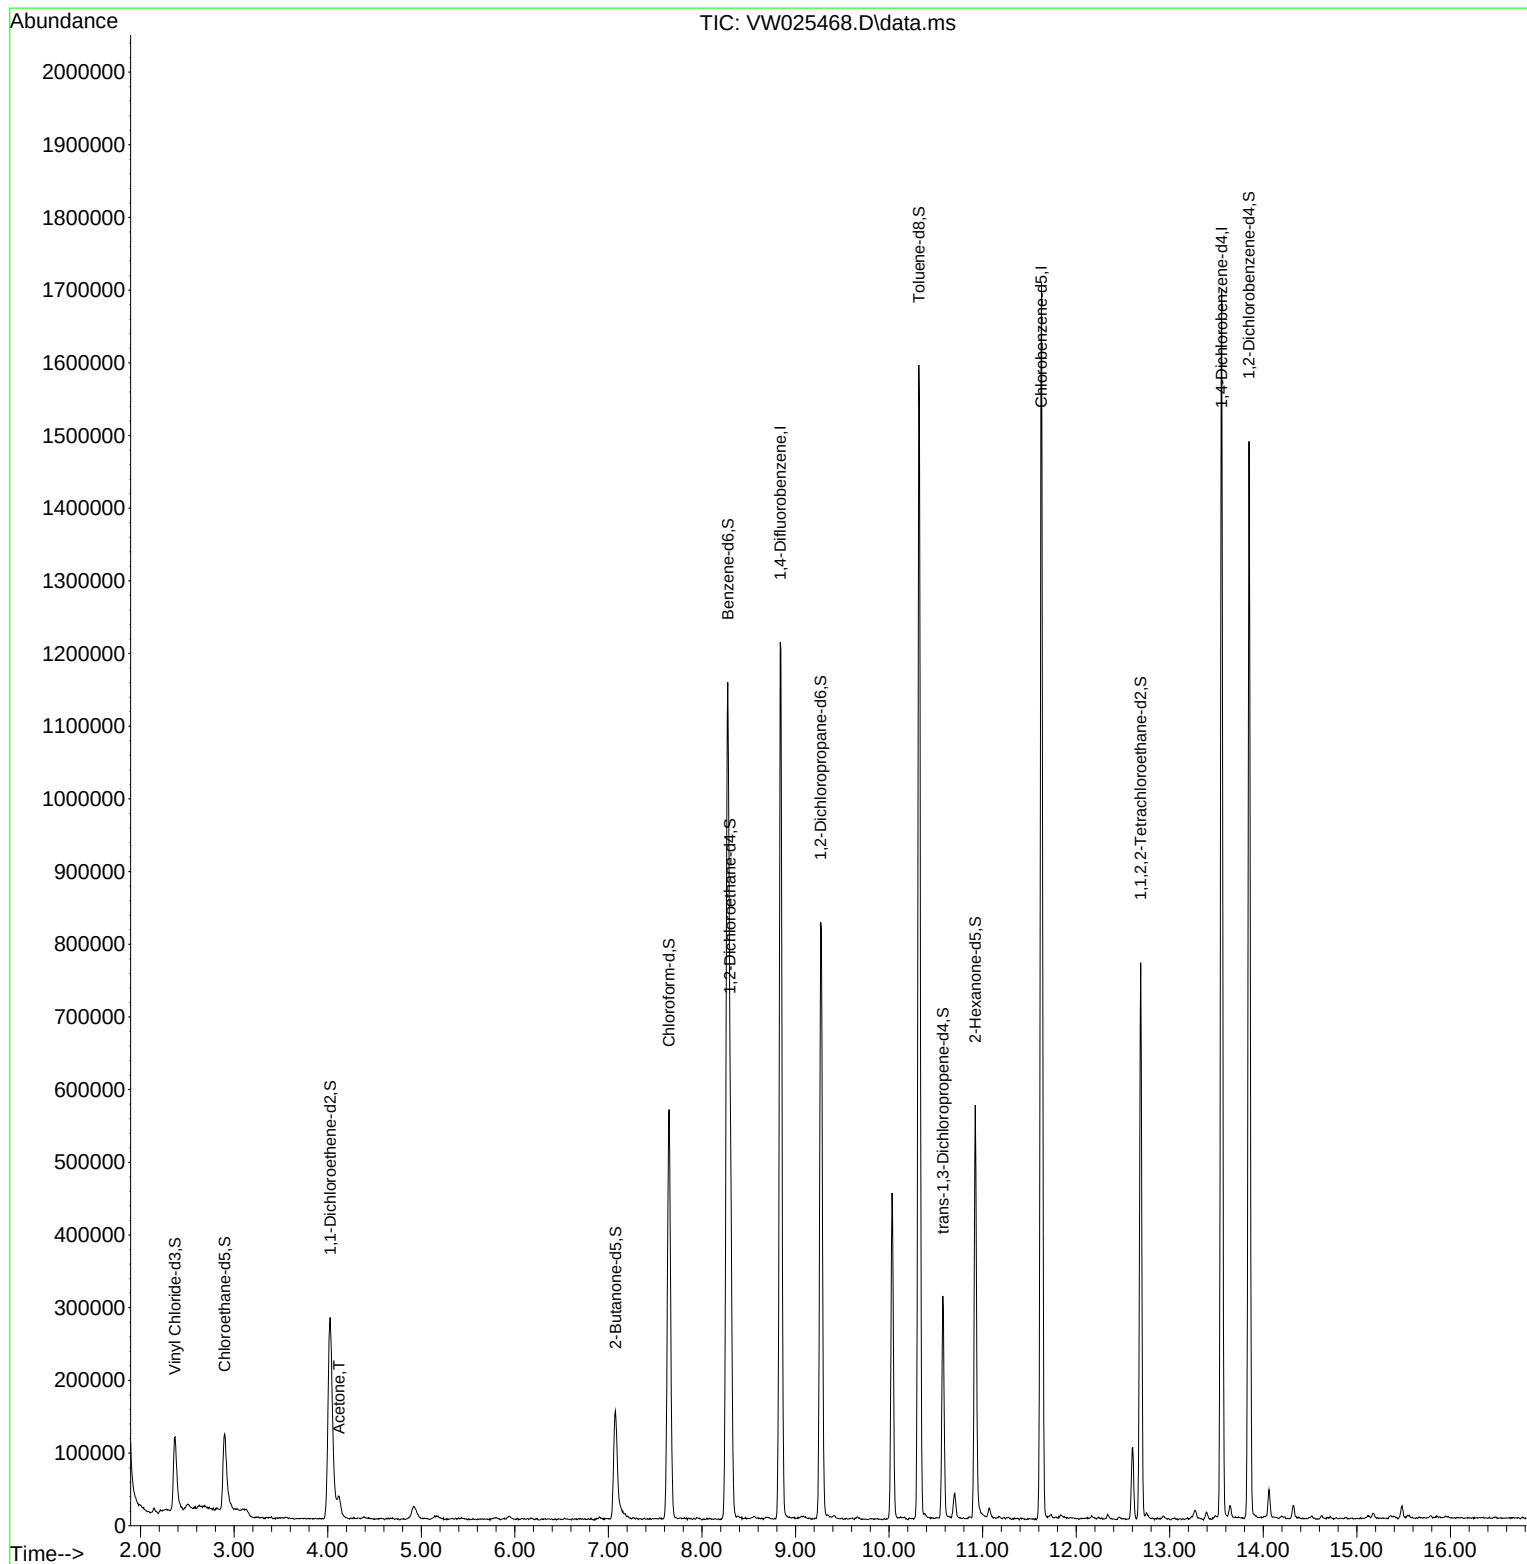

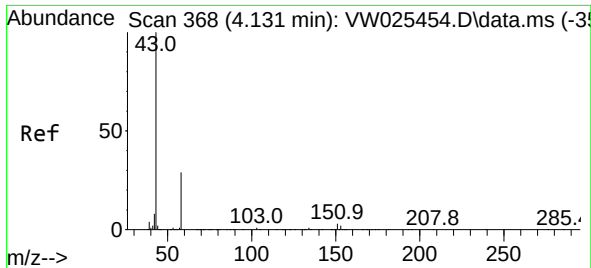

#13
 Acetone
 Concen: 11.900 ug/L
 RT: 4.118 min Scan# 30
 Delta R.T. -0.012 min
 Lab File: VW025468.D
 Acq: 21 Mar 2023 15:04

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGC1

Tgt Ion: 43 Resp: 44526
 Ion Ratio Lower Upper
 43 100
 58 29.3 0.0 60.0

