
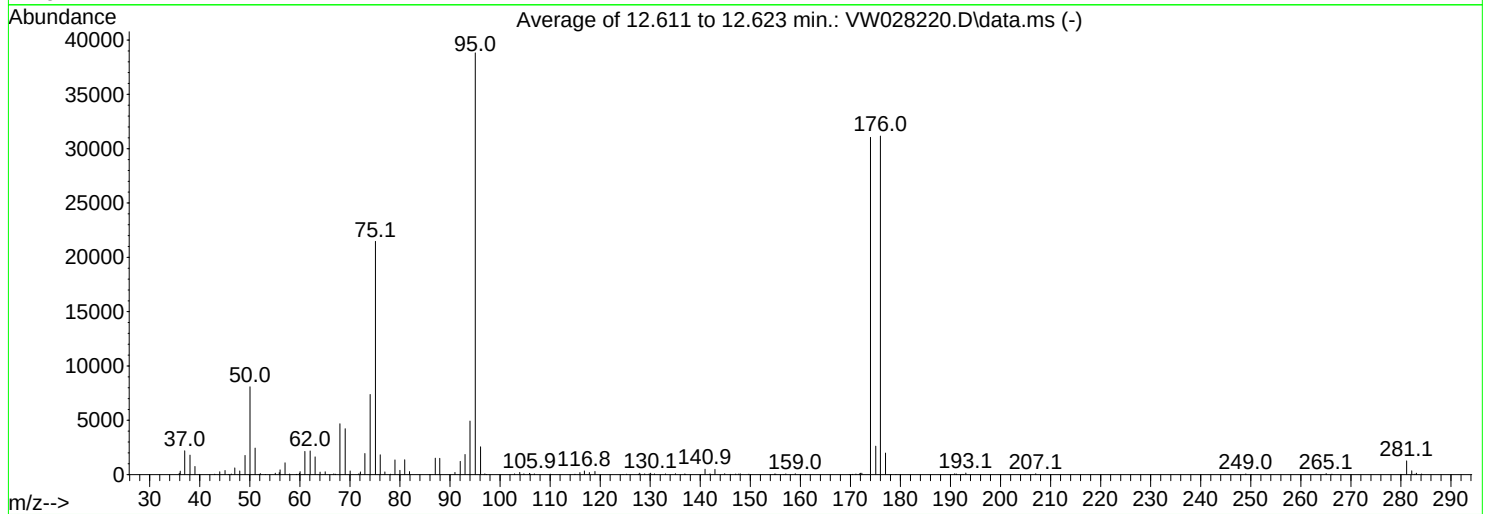


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032124\
Data File : VW028220.D
Acq On : 21 Mar 2024 08:23
Operator : SY/MD
Sample : BFB456
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB456

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Title : SFAM01.0
Last Update : Fri Mar 22 01:31:33 2024

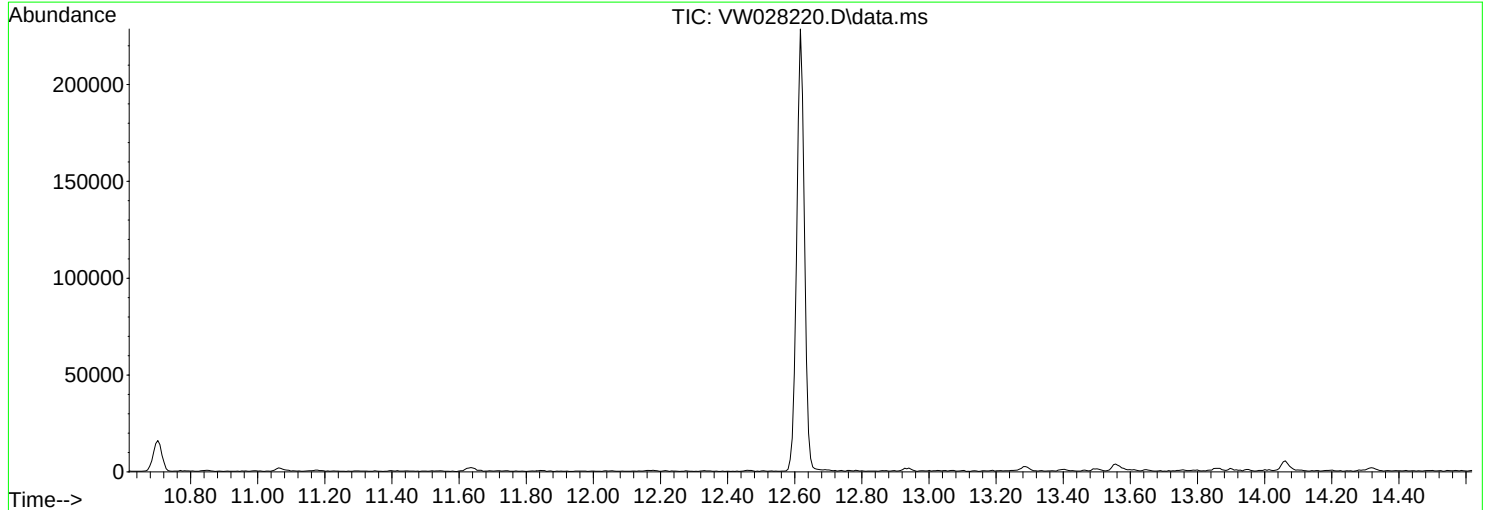

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	8090	PASS
75	95	30	80	55.3	21467	PASS
95	95	100	100	100.0	38821	PASS
96	95	5	9	6.6	2557	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.0	31051	PASS
175	174	5	9	8.5	2626	PASS
176	174	95	101	100.4	31160	PASS
177	176	5	9	6.4	1989	PASS

m/z	Abundance
37.60	64.0
39.90	145.0
40.90	50.0
44.00	78.0
47.70	51.0
57.20	61.0

Instrument :
MSVOA_W
ClientSampleId :
BFB456

m/z	Abundance
35.90	394.0
37.00	2104.0
38.00	1640.0
39.00	826.0
40.10	159.0
44.10	409.0
45.10	352.0
46.30	99.0
47.00	656.0
48.10	310.0
49.10	1678.0
50.10	7843.0
51.00	2370.0
52.20	166.0
53.10	50.0
55.10	150.0
55.90	597.0
57.00	1040.0
58.00	60.0
59.30	89.0
59.90	406.0
61.00	1861.0
62.10	2160.0
63.10	1454.0
64.10	286.0
65.10	239.0
66.90	116.0
68.00	4363.0
69.10	3736.0
70.10	237.0
72.00	270.0
73.00	1933.0
74.00	7108.0
75.10	19616.0
76.10	1580.0
77.00	356.0
79.00	1180.0
80.10	316.0
81.00	1226.0
81.90	239.0
87.00	1277.0
87.90	1449.0
91.10	174.0
92.10	1186.0
93.00	1610.0
94.00	4497.0
95.00	35568.0
96.10	2565.0
97.00	72.0
97.30	64.0
103.00	107.0
103.90	149.0
104.70	88.0
105.90	174.0
106.80	51.0
110.10	74.0
114.90	68.0
116.00	186.0
116.80	349.0
118.00	176.0
119.00	296.0
124.60	60.0
125.30	133.0
127.70	150.0
128.90	77.0
129.80	75.0
130.20	84.0
130.80	62.0
133.10	164.0
135.10	63.0
136.80	68.0
137.10	70.0
140.90	482.0
141.90	95.0
143.00	413.0
144.90	92.0
146.10	58.0
147.10	65.0
147.70	119.0
154.90	93.0
157.10	62.0
159.00	137.0
171.80	241.0
174.00	25632.0
175.00	2235.0
176.00	24496.0
177.00	1810.0
178.10	68.0
179.10	53.0
190.80	123.0
191.20	161.0
192.30	110.0

Instrument :
MSVOA_W
ClientSampleId :
BFB456

193.00	254.0
204.90	52.0
207.00	126.0
249.10	130.0
250.10	56.0
265.10	235.0
266.30	77.0
281.20	2061.0
282.20	519.0
283.10	398.0
284.20	108.0

Instrument :
MSVOA_W
ClientSampleId :
BFB456

m/z	Abundance
36.10	541.0
37.00	2706.0
38.10	2038.0
39.10	737.0
40.10	161.0
43.00	52.0
44.00	367.0
45.00	441.0
45.80	102.0
46.30	63.0
46.90	669.0
47.90	380.0
49.00	1945.0
50.10	8832.0
51.10	2677.0
52.10	109.0
55.10	154.0
56.10	725.0
57.10	1332.0
57.90	111.0
60.10	372.0
61.00	2547.0
62.00	2490.0
63.00	2009.0
64.00	212.0
65.10	310.0
66.70	111.0
68.00	5202.0
69.00	4989.0
70.00	414.0
72.10	277.0
73.00	2181.0
74.00	8550.0
75.10	25168.0
76.00	2263.0
77.10	150.0
79.00	1438.0
80.00	531.0
81.00	1494.0
82.00	296.0
86.00	70.0
87.00	1984.0
87.90	1656.0
90.90	218.0
92.00	1393.0
93.00	2077.0
94.00	5475.0
95.10	44392.0
96.10	2882.0
96.90	142.0
102.90	55.0
104.00	245.0
104.80	130.0
106.10	151.0
106.80	95.0
110.00	80.0
115.00	61.0
116.00	186.0
116.90	346.0
117.80	234.0
118.90	322.0
127.90	197.0
129.80	136.0
130.10	123.0
130.80	120.0
133.00	69.0
135.10	133.0
136.90	115.0
141.00	466.0
142.00	68.0
143.00	501.0
144.90	167.0
145.90	53.0
147.10	130.0
147.70	83.0
148.10	89.0
149.80	61.0
154.80	101.0
157.10	79.0
159.00	95.0
161.10	50.0
170.40	73.0
171.10	103.0
172.00	385.0
174.00	35024.0
175.00	2996.0
176.00	35304.0
177.00	2318.0
190.90	110.0
192.60	59.0
193.10	131.0
207.10	165.0

Instrument :
MSVOA_W
ClientSampleId :
BFB456

248.90	83.0
265.00	87.0
266.10	62.0
280.00	79.0
281.00	969.0
282.20	328.0
282.80	159.0
284.10	56.0

Instrument :
MSVOA_W
ClientSampleId :
BFB456

m/z	Abundance
36.10	429.0
37.00	1779.0
38.10	1737.0
39.10	692.0
40.00	195.0
43.00	67.0
43.90	271.0
45.00	353.0
47.10	525.0
48.00	332.0
49.10	1671.0
50.00	7595.0
51.00	2271.0
51.90	122.0
55.10	106.0
56.00	615.0
57.10	1062.0
60.00	450.0
61.00	2008.0
62.10	1875.0
63.10	1464.0
64.10	229.0
64.90	262.0
67.10	142.0
68.00	4507.0
69.10	3963.0
70.00	359.0
71.80	267.0
72.20	227.0
73.00	1704.0
74.10	6496.0
75.10	19616.0
76.10	1649.0
76.90	227.0
78.10	138.0
79.00	1451.0
79.90	332.0
80.90	1378.0
81.80	309.0
87.10	1313.0
88.00	1385.0
91.00	220.0
92.10	1110.0
93.00	1877.0
94.00	4823.0
95.10	36504.0
96.10	2225.0
102.80	68.0
104.00	226.0
105.90	200.0
106.90	57.0
115.90	195.0
116.90	326.0
117.80	185.0
119.00	253.0
127.90	200.0
128.90	126.0
130.00	193.0
130.90	62.0
135.00	73.0
137.10	77.0
141.00	538.0
142.00	61.0
142.90	534.0
147.90	125.0
149.60	55.0
155.10	168.0
156.70	67.0
157.10	78.0
159.00	56.0
161.00	59.0
169.80	52.0
171.10	59.0
172.30	396.0
174.00	32496.0
175.10	2648.0
176.00	33680.0
177.00	1838.0
190.80	54.0
193.10	61.0
281.10	766.0
282.00	211.0

Instrument :
MSVOA_W
ClientSampleId :
BFB456