




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032224\
Data File : VW028233.D
Acq On : 22 Mar 2024 17:25
Operator : SY/MD
Sample : P1839-10
Misc : 4.14g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOLY8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/25/2024
Supervised By :Mahesh Dadoda 03/25/2024

Quant Time: Mar 23 01:02:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Mar 23 01:00:21 2024
Response via : Initial Calibration

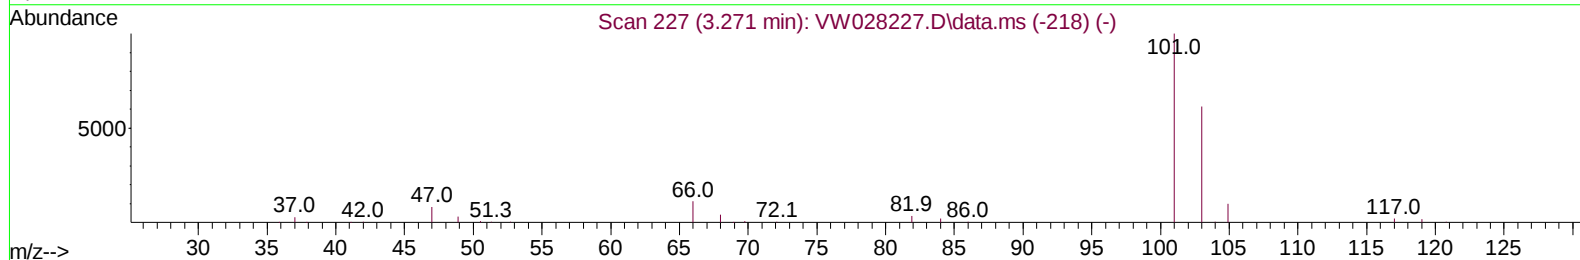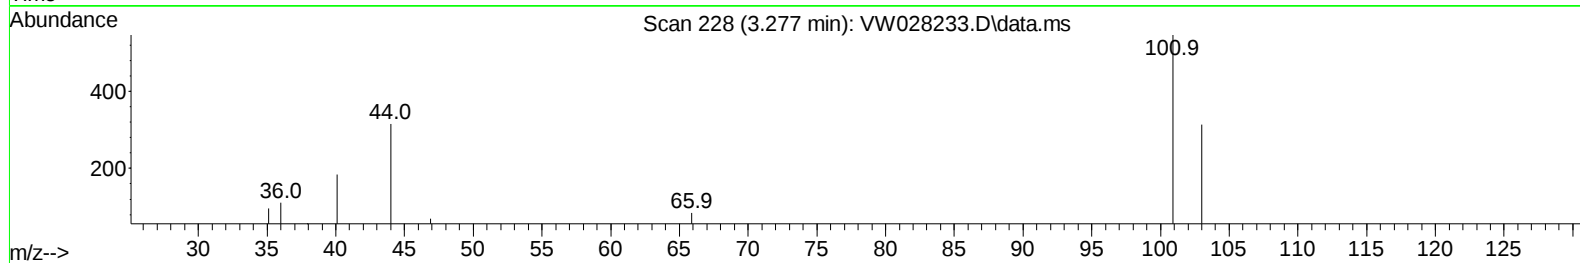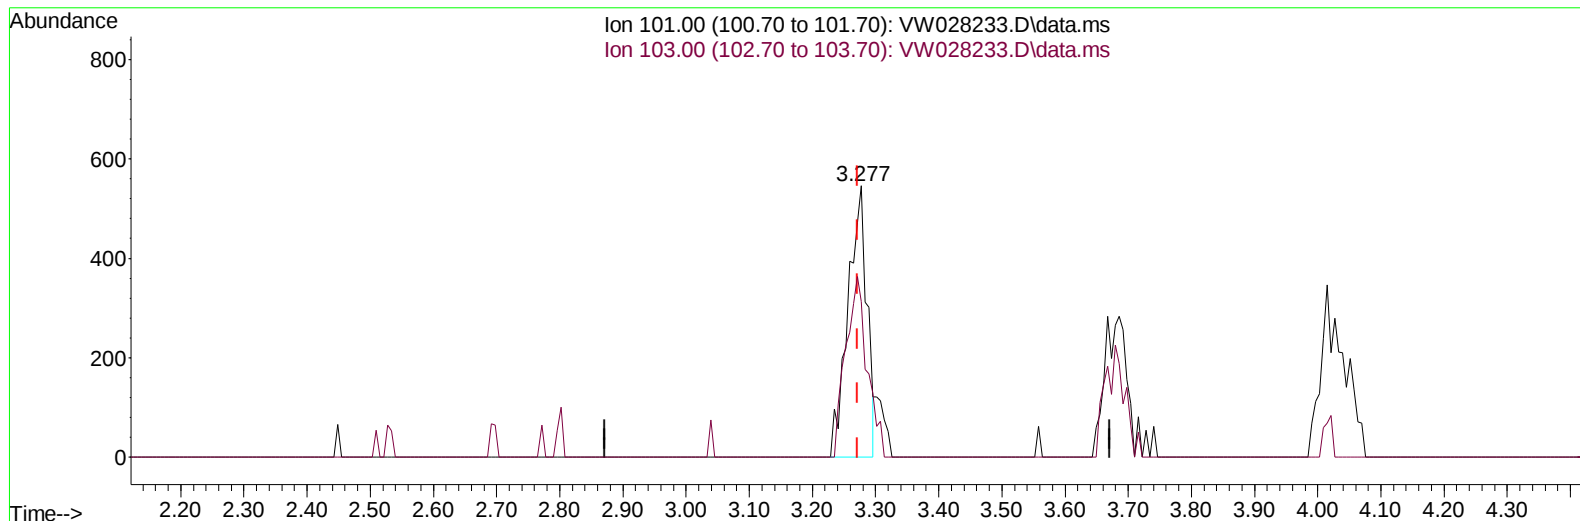

TIC: VW028233.D\data.ms

(9) Trichlorofluoromethane (T)

3.277min (+ 0.006) 0.37 ug/L

response 1137

Ion	Exp%	Act%
101.00	100.00	100.00
103.00	63.60	75.90
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032224\
 Data File : VW028233.D
 Acq On : 22 Mar 2024 17:25
 Operator : SY/MD
 Sample : P1839-10
 Misc : 4.14g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOLY8

Manual IntegrationsAPPROVED

Quant Time: Mar 23 01:02:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Mar 23 01:00:21 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/25/2024
 Supervised By :Mahesh Dadoda 03/25/2024

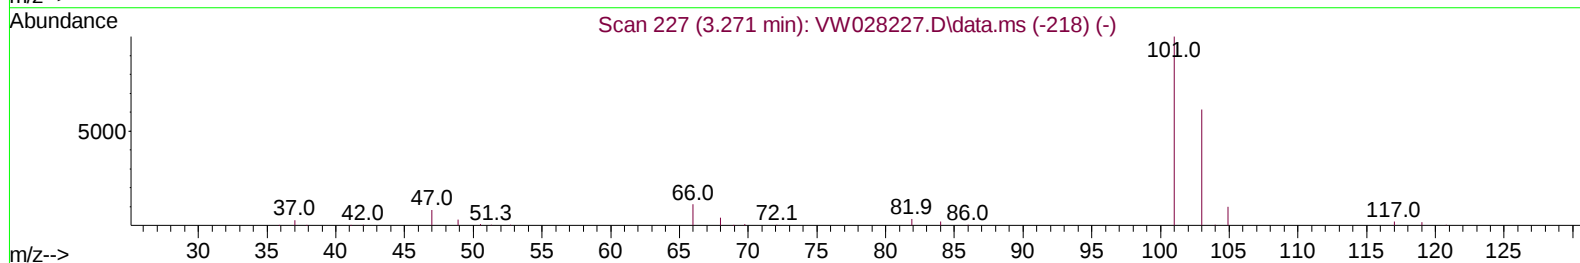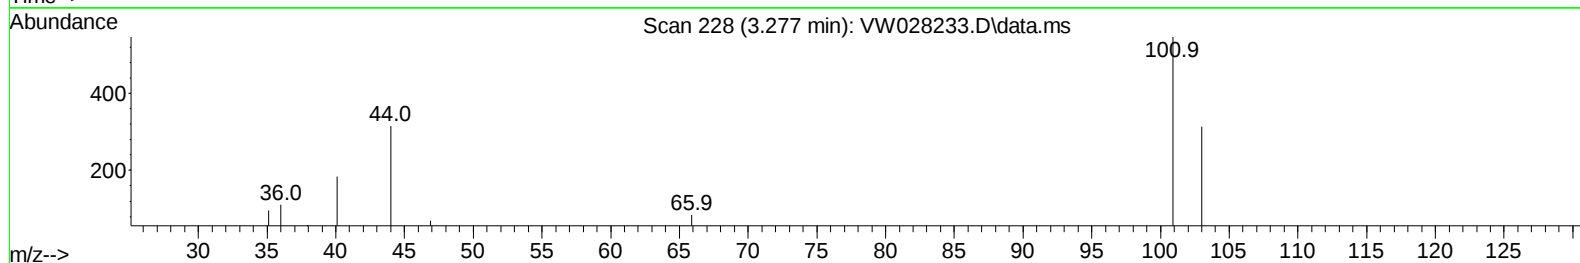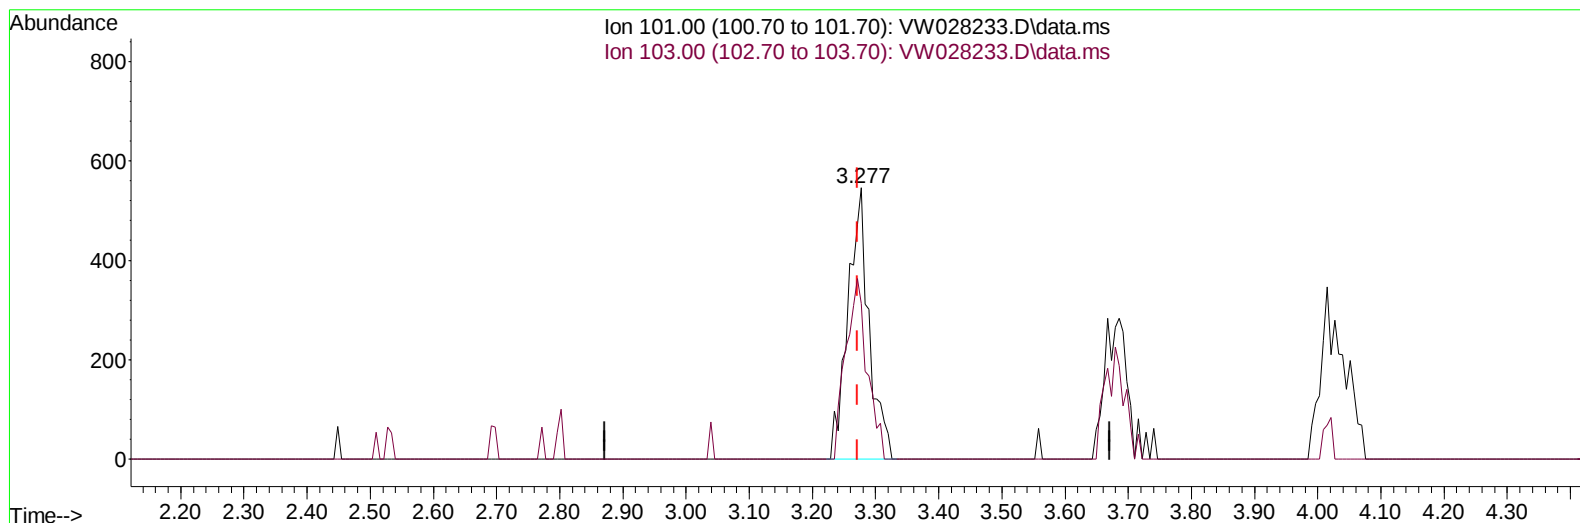

TIC: VW028233.D\data.ms

(9) Trichlorofluoromethane (T)

3.277min (+ 0.006) 0.41 ug/L m

response 1270

Ion	Exp%	Act%
101.00	100.00	100.00
103.00	63.60	67.95
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032224\
 Data File : VW028233.D
 Acq On : 22 Mar 2024 17:25
 Operator : SY/MD
 Sample : P1839-10
 Misc : 4.14g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E0LY8

Manual IntegrationsAPPROVED

Quant Time: Mar 23 01:02:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Mar 23 01:00:21 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/25/2024
 Supervised By :Mahesh Dadoda 03/25/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		218008	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		148259	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		41636	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		43174	16.926	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	67.720%		
7) Chloroethane-d5	2.905	69		33563	18.833	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	75.320%		
11) 1,1-Dichloroethene-d2	4.021	65		26617	16.455	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	65.800%		
21) 2-Butanone-d5	7.081	46		27520	36.580	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	73.160%		
24) Chloroform-d	7.648	84		118139	18.377	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	73.520%		
26) 1,2-Dichloroethane-d4	8.307	65		70843	19.997	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	80.000%		
32) Benzene-d6	8.276	84		216791	23.950	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	95.800%		
36) 1,2-Dichloropropane-d6	9.276	67		67157	25.781	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	103.120%		
41) Toluene-d8	10.325	98		164038	19.647	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	78.600%		
43) trans-1,3-Dichloroprop...	10.575	79		23969	20.259	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	81.040%		
47) 2-Hexanone-d5	10.922	63		18794	43.648	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	87.300%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		41283	21.455	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	85.800%		
66) 1,2-Dichlorobenzene-d4	13.848	152		29570	19.496	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	78.000%		
Target Compounds							
9) Trichlorofluoromethane	3.277	101		1270m	0.414	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032224\
Data File : VW028233.D
Acq On : 22 Mar 2024 17:25
Operator : SY/MD
Sample : P1839-10
Misc : 4.14g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E0LY8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/25/2024
Supervised By :Mahesh Dadoda 03/25/2024

Quant Time: Mar 23 01:02:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Mar 23 01:00:21 2024
Response via : Initial Calibration

