

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032224\
 Data File : VW028229.D
 Acq On : 22 Mar 2024 15:50
 Operator : SY/MD
 Sample : P1839-07
 Misc : 4.45g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E0LY5

Quant Time: Mar 23 01:00:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Mar 23 01:00:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	253305	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	202620	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	74316	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	40171	13.554	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	54.200%
7) Chloroethane-d5	2.899	69	31195	15.065	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.280%
11) 1,1-Dichloroethene-d2	4.027	65	27862	14.824	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	59.280%
21) 2-Butanone-d5	7.081	46	26480	30.293	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	60.580%
24) Chloroform-d	7.654	84	121397	16.253	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	65.000%
26) 1,2-Dichloroethane-d4	8.306	65	66541	16.166	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	64.680%#
32) Benzene-d6	8.276	84	230395	18.624	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	74.480%
36) 1,2-Dichloropropane-d6	9.276	67	68357	19.201	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	76.800%
41) Toluene-d8	10.324	98	193826	16.987	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	67.960%
43) trans-1,3-Dichloroprop...	10.574	79	26629	16.469	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	65.880%
47) 2-Hexanone-d5	10.922	63	20889	35.498	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.000%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	44515	16.927	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	67.720%
66) 1,2-Dichlorobenzene-d4	13.848	152	44773	16.538	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	66.160%#
Target Compounds					Qvalue	
13) Acetone	4.143	43	4630	4.770	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032224\
Data File : VW028229.D
Acq On : 22 Mar 2024 15:50
Operator : SY/MD
Sample : P1839-07
Misc : 4.45g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOLY5

Quant Time: Mar 23 01:00:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Mar 23 01:00:21 2024
Response via : Initial Calibration

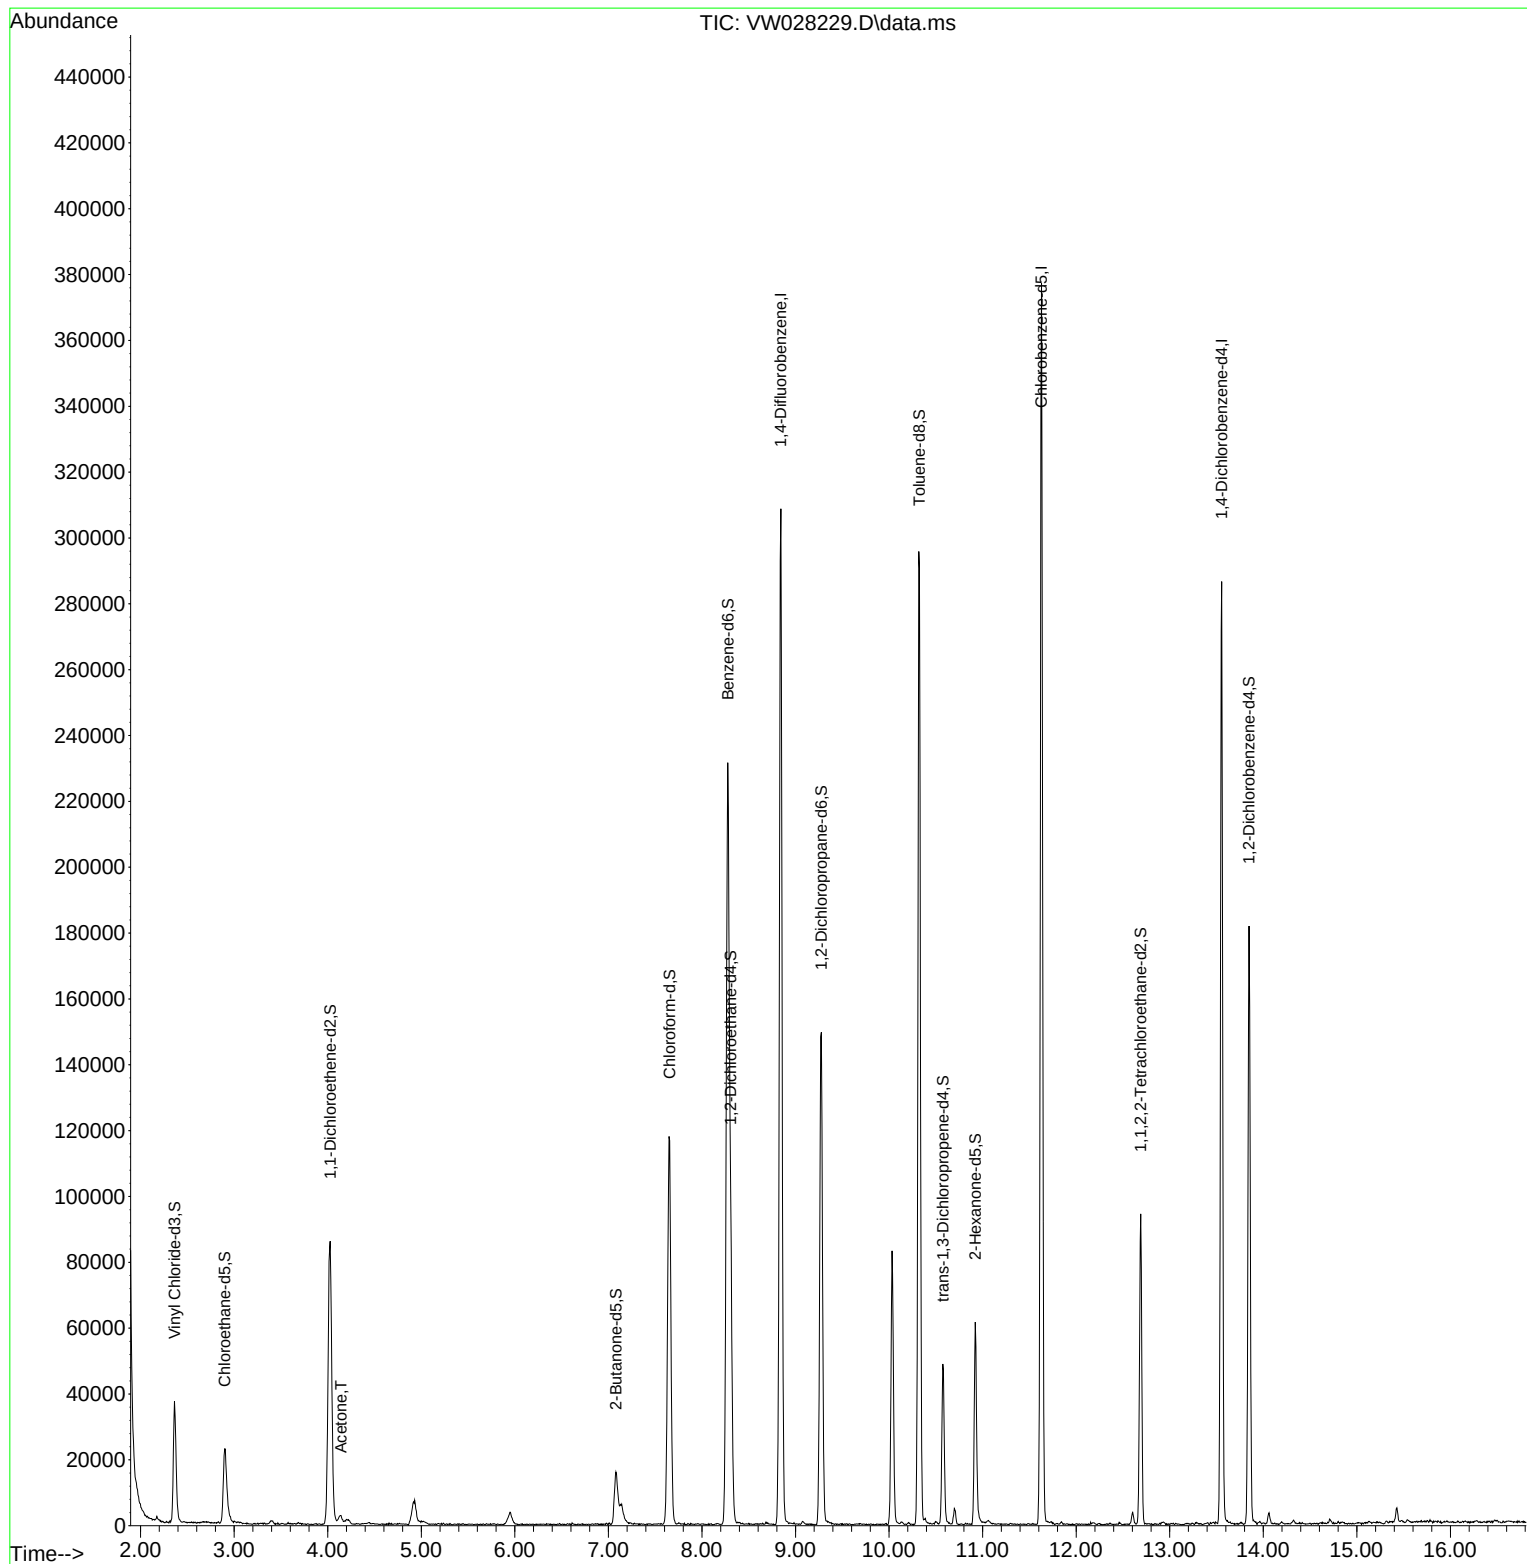

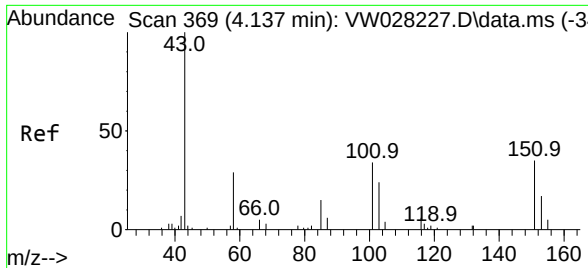

#13
 Acetone
 Concen: 4.770 ug/L
 RT: 4.143 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: VW028229.D
 Acq: 22 Mar 2024 15:50

Instrument :
 MSVOA_W
 ClientSampleId :
 E0LY5

Tgt Ion: 43 Resp: 4630
 Ion Ratio Lower Upper
 43 100
 58 31.0 0.0 57.8

