
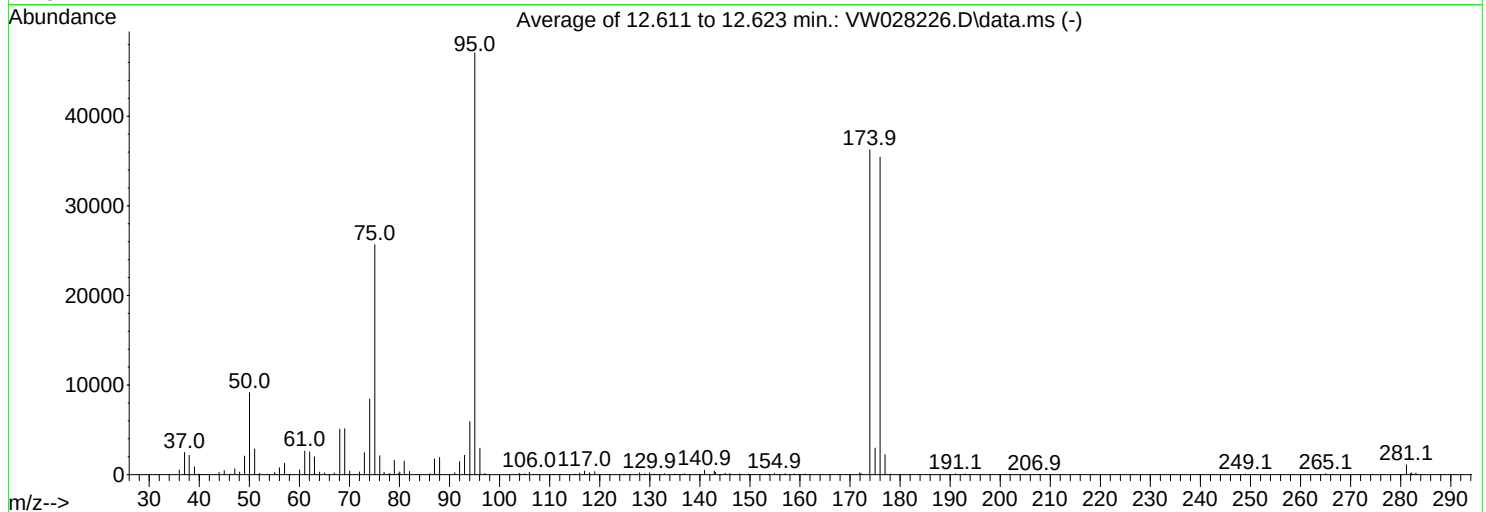


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032224\
Data File : VW028226.D
Acq On : 22 Mar 2024 13:53
Operator : SY/MD
Sample : BFB457
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB457

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Title : SFAM01.0
Last Update : Tue Mar 26 01:17:39 2024

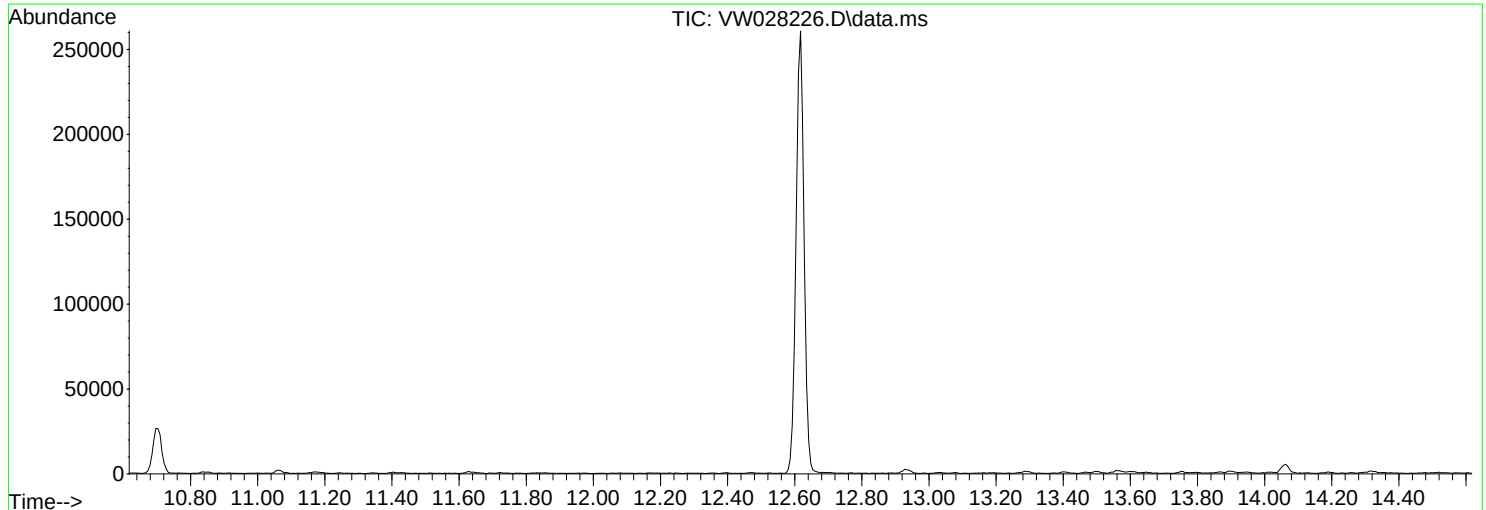

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.4	9156	PASS
75	95	30	80	54.5	25667	PASS
95	95	100	100	100.0	47080	PASS
96	95	5	9	6.3	2945	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.0	36253	PASS
175	174	5	9	8.2	2963	PASS
176	174	95	101	97.7	35432	PASS
177	176	5	9	6.3	2239	PASS

m/z	Abundance
40.00	142.0
43.90	143.0
56.30	61.0

Instrument :
MSVOA_W
ClientSampleId :
BFB457

m/z	Abundance
36.00	479.0
37.10	2713.0
38.00	2291.0
39.00	861.0
40.00	333.0
40.60	52.0
41.30	54.0
44.00	489.0
45.00	500.0
46.20	78.0
47.00	650.0
48.00	301.0
49.00	2169.0
50.00	10113.0
51.10	3030.0
52.00	137.0
55.10	214.0
56.10	792.0
57.10	1266.0
58.00	90.0
60.10	647.0
61.00	2680.0
62.00	2720.0
63.00	2176.0
64.00	255.0
65.10	192.0
67.00	201.0
68.10	5088.0
69.00	5390.0
70.10	490.0
71.10	52.0
72.10	263.0
73.00	2557.0
74.00	8730.0
75.10	26688.0
76.00	1969.0
76.90	172.0
77.90	251.0
79.00	1661.0
79.80	390.0
80.90	1551.0
82.00	323.0
86.00	86.0
87.00	1843.0
88.00	1914.0
89.10	51.0
91.00	273.0
92.00	1389.0
93.00	2129.0
94.10	5908.0
95.10	47504.0
96.10	3056.0
97.00	140.0
104.00	229.0
105.10	119.0
105.90	194.0
106.80	66.0
110.80	99.0
111.80	57.0
115.00	60.0
116.00	204.0
116.90	396.0
117.90	202.0
119.00	355.0
124.90	133.0
128.00	187.0
129.00	110.0
129.90	225.0
130.90	89.0
132.90	238.0
133.80	57.0
135.00	84.0
136.50	58.0
137.00	129.0
141.00	448.0
142.90	647.0
144.40	63.0
145.00	233.0
146.00	102.0
147.00	54.0
147.70	106.0
149.70	51.0
154.90	134.0
157.00	153.0
158.80	66.0
161.00	183.0
171.90	287.0
174.00	34952.0
175.00	2729.0
176.00	31488.0
177.00	2312.0
191.10	183.0

Instrument :
MSVOA_W
ClientSampleId :
BFB457

192.90	144.0
193.70	61.0
249.10	126.0
251.00	71.0
265.10	181.0
281.10	1658.0
282.20	578.0
283.10	285.0
284.20	68.0

Instrument :
MSVOA_W
ClientSampleId :
BFB457

m/z	Abundance
36.00	579.0
37.10	2584.0
38.00	2584.0
39.00	920.0
39.90	131.0
43.10	68.0
43.90	415.0
45.00	495.0
46.20	66.0
47.10	832.0
48.10	293.0
49.10	2287.0
50.10	9902.0
51.00	3064.0
52.00	161.0
55.10	345.0
55.90	873.0
57.00	1530.0
58.20	130.0
60.00	651.0
61.10	2618.0
62.10	2933.0
63.00	2377.0
64.00	365.0
65.00	166.0
67.00	193.0
68.00	5986.0
69.00	5951.0
70.00	442.0
71.90	376.0
73.00	2786.0
74.00	9247.0
75.00	27944.0
76.00	2399.0
76.90	300.0
78.10	206.0
78.90	1724.0
80.00	546.0
80.90	1672.0
82.00	463.0
86.10	119.0
87.00	1799.0
88.00	2152.0
91.00	199.0
92.00	1811.0
93.00	2494.0
94.10	6761.0
95.10	52624.0
96.10	3215.0
97.10	132.0
103.80	240.0
105.00	101.0
106.00	309.0
106.80	54.0
111.00	77.0
112.10	84.0
115.20	89.0
115.90	175.0
117.00	451.0
118.00	232.0
119.00	360.0
124.80	60.0
127.90	236.0
129.00	104.0
130.00	203.0
130.90	97.0
132.90	129.0
134.80	116.0
136.50	57.0
136.90	147.0
139.50	54.0
141.00	559.0
143.10	731.0
144.00	79.0
145.10	173.0
146.00	152.0
148.00	142.0
149.80	84.0
153.70	57.0
154.80	202.0
157.10	110.0
158.90	96.0
161.10	87.0
172.00	373.0
174.00	38872.0
175.00	3277.0
176.00	40008.0
177.00	2269.0
178.00	79.0
191.10	143.0
193.10	147.0
206.90	58.0

Instrument :
MSVOA_W
ClientSampleId :
BFB457

249.00	69.0
250.80	64.0
265.00	120.0
281.20	1124.0
281.90	263.0
283.00	254.0

Instrument :
MSVOA_W
ClientSampleId :
BFB457

m/z	Abundance
36.00	478.0
37.00	2136.0
38.00	1595.0
39.10	853.0
39.90	177.0
44.10	261.0
45.00	368.0
47.20	524.0
48.00	270.0
49.00	1774.0
50.10	7453.0
51.00	2490.0
52.10	141.0
55.10	205.0
56.00	662.0
57.00	1025.0
58.10	72.0
60.00	307.0
61.00	2555.0
62.10	1930.0
63.00	1411.0
64.10	215.0
65.10	238.0
65.90	54.0
66.90	178.0
68.10	4153.0
69.10	4058.0
70.00	325.0
72.00	261.0
73.00	2023.0
74.10	7290.0
75.10	22368.0
76.10	1959.0
76.90	314.0
78.10	138.0
78.90	1397.0
80.10	353.0
81.00	1327.0
82.00	265.0
83.30	67.0
86.20	95.0
87.00	1670.0
88.00	1666.0
91.10	166.0
92.00	1178.0
93.00	1891.0
94.00	5104.0
95.00	41112.0
96.00	2563.0
97.10	96.0
104.10	161.0
105.00	99.0
105.90	302.0
111.70	56.0
115.00	91.0
115.90	137.0
116.90	350.0
118.00	200.0
119.00	289.0
127.90	182.0
129.10	50.0
129.90	213.0
130.90	54.0
135.10	89.0
135.70	62.0
136.90	59.0
139.40	60.0
140.90	476.0
142.90	564.0
144.90	80.0
145.30	81.0
146.00	114.0
147.90	121.0
149.80	60.0
153.70	66.0
155.00	118.0
157.10	101.0
158.90	83.0
172.20	387.0
173.90	34936.0
175.00	2883.0
176.00	34800.0
177.00	2136.0
178.10	134.0
193.00	73.0
281.10	514.0
282.00	107.0
282.50	53.0
283.40	88.0

Instrument :
MSVOA_W
ClientSampleId :
BFB457