

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032319\
Quantitation Report (QT Reviewed)


Data File : VW009402.D
Acq On : 23 Mar 2019 21:11
Operator : SY/VA
Sample : K2062-18
Misc : 4.20G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF0H5

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:33:36 AM

Quant Time: Mar 24 00:31:38 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 23:52:05 2019
Response via : Initial Calibration

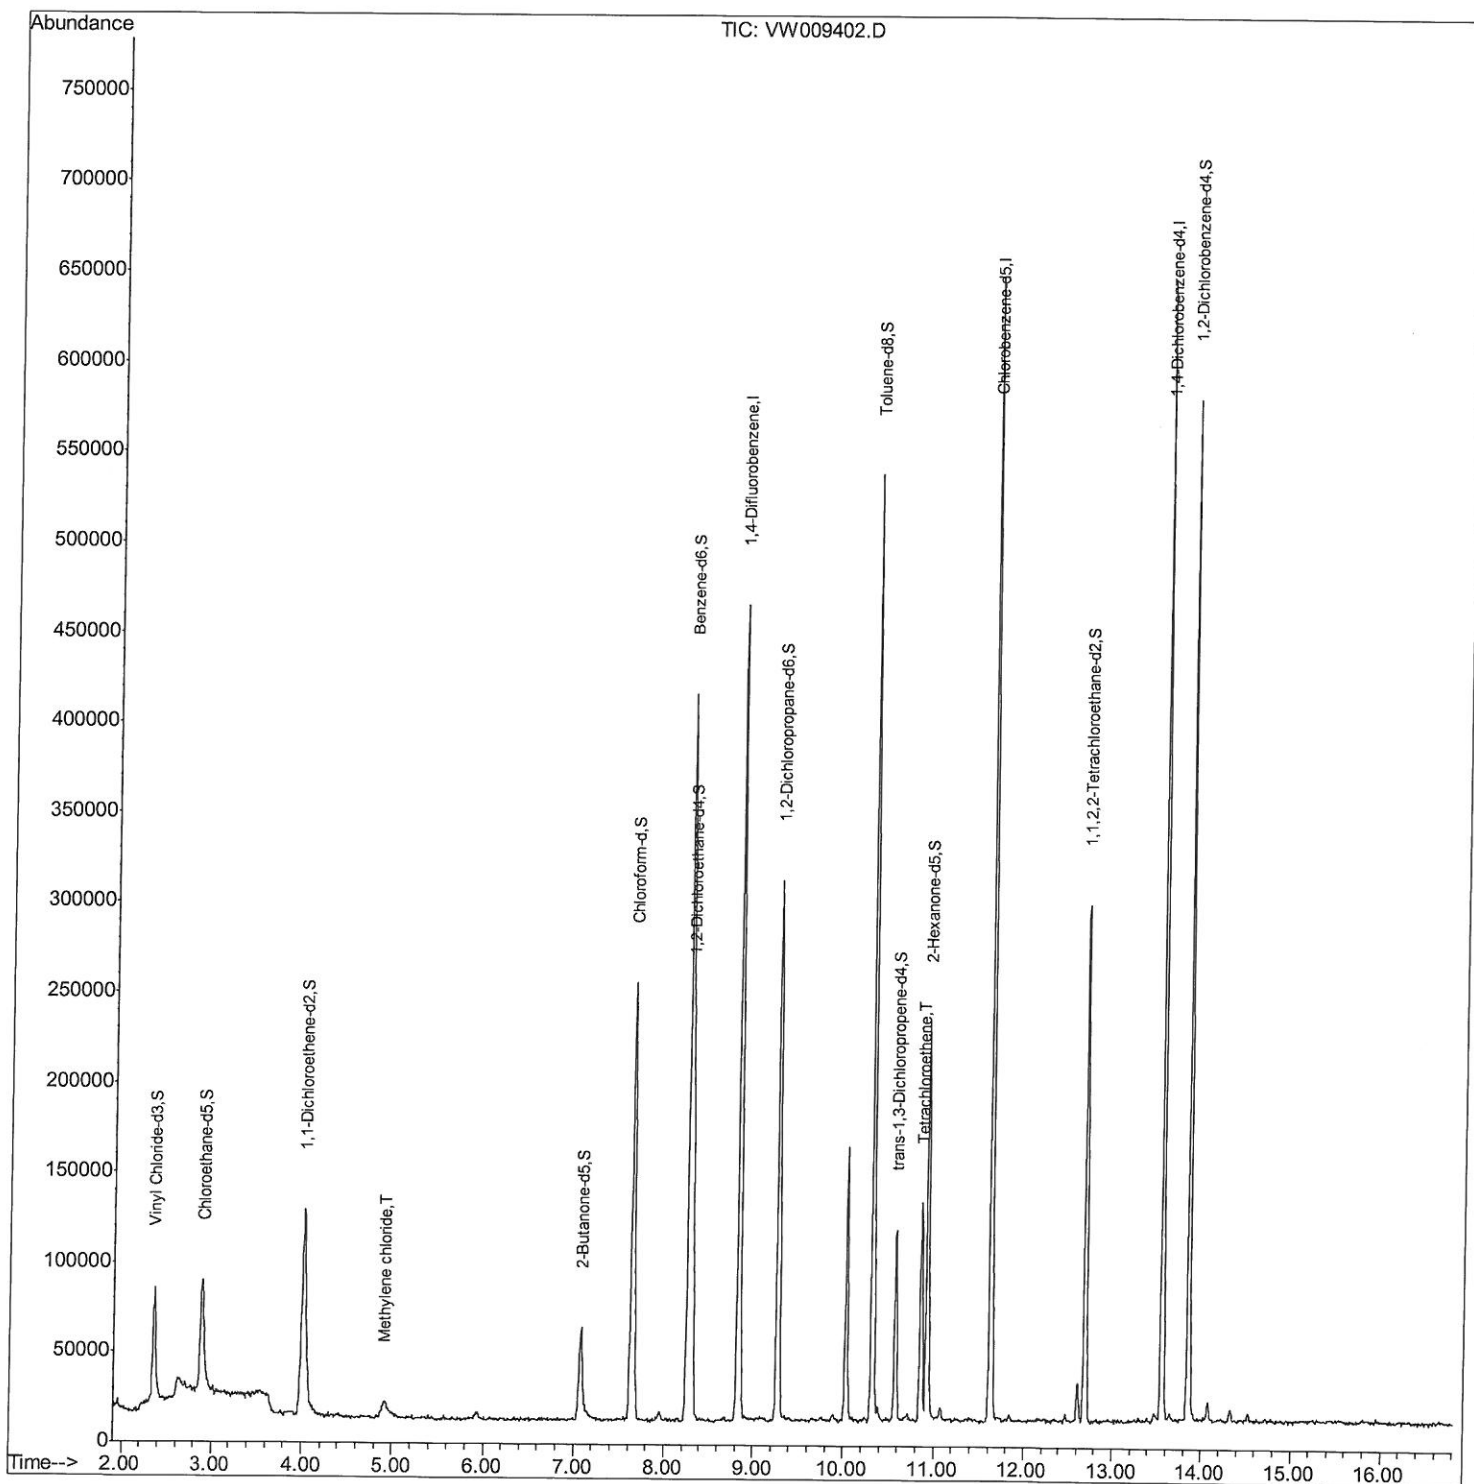

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032319\
Quantitation Report (Qedit)




Data File : VW009402.D
Acq On : 23 Mar 2019 21:11
Operator : SY/VA
Sample : K2062-18
Misc : 4.20G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF0H5

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:33:36 AM

Quant Time: Mar 23 23:56:36 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 23:52:05 2019
Response via : Initial Calibration

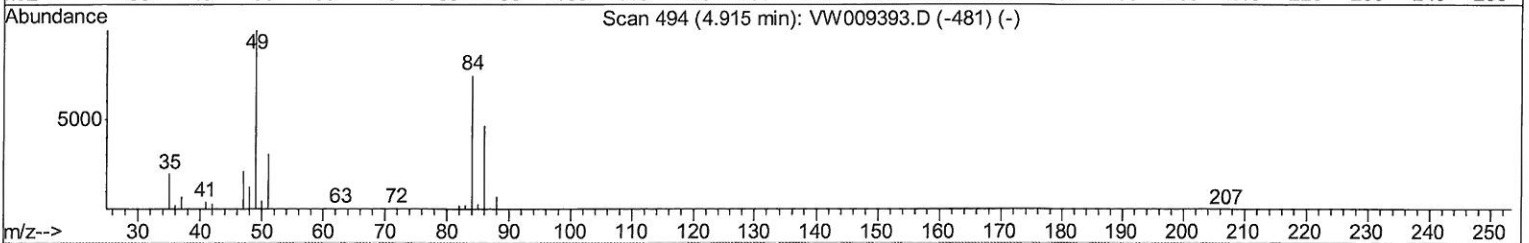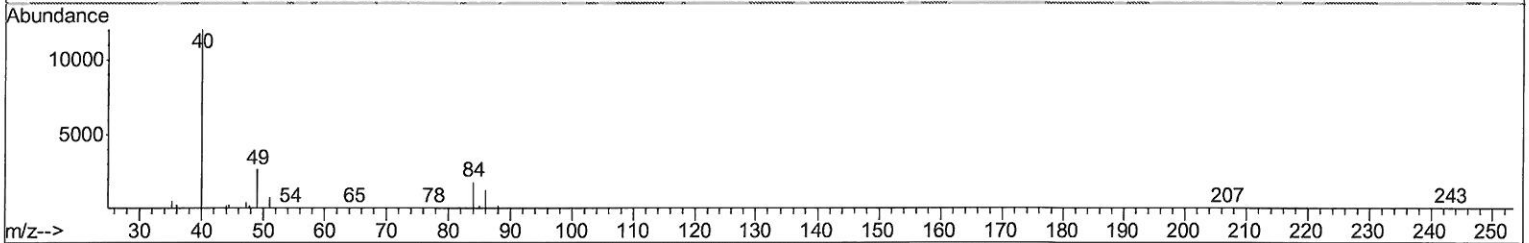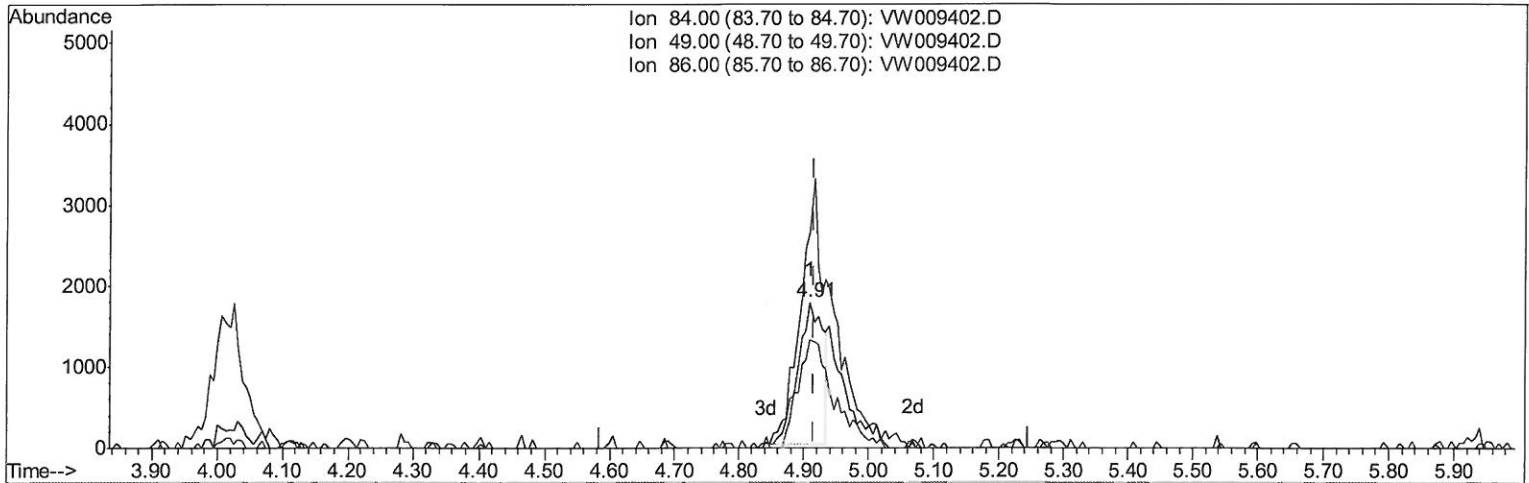

TIC: VW009402.D

(16) Methylene chloride (T)

4.909min (-0.006) 0.92ug/L

response 4702

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	149.13
86.00	63.50	74.54
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032319\
Quantitation Report (Qedit)




Data File : VW009402.D
Acq On : 23 Mar 2019 21:11
Operator : SY/VA
Sample : K2062-18
Misc : 4.20G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF0H5

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:33:36 AM

Quant Time: Mar 23 23:56:36 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 23:52:05 2019
Response via : Initial Calibration

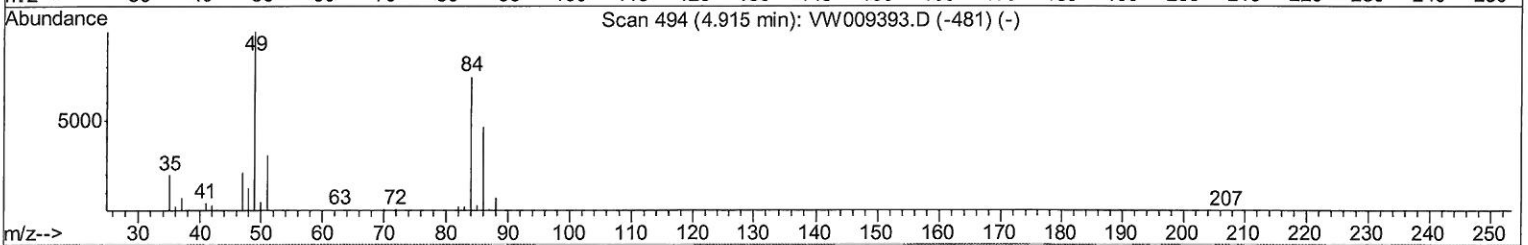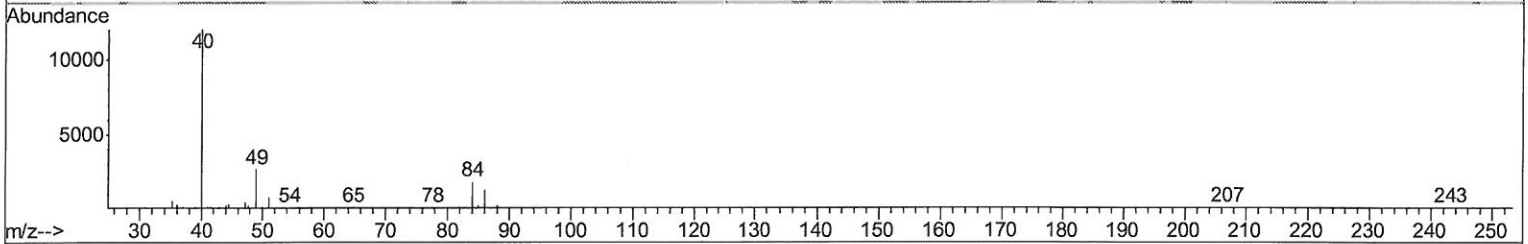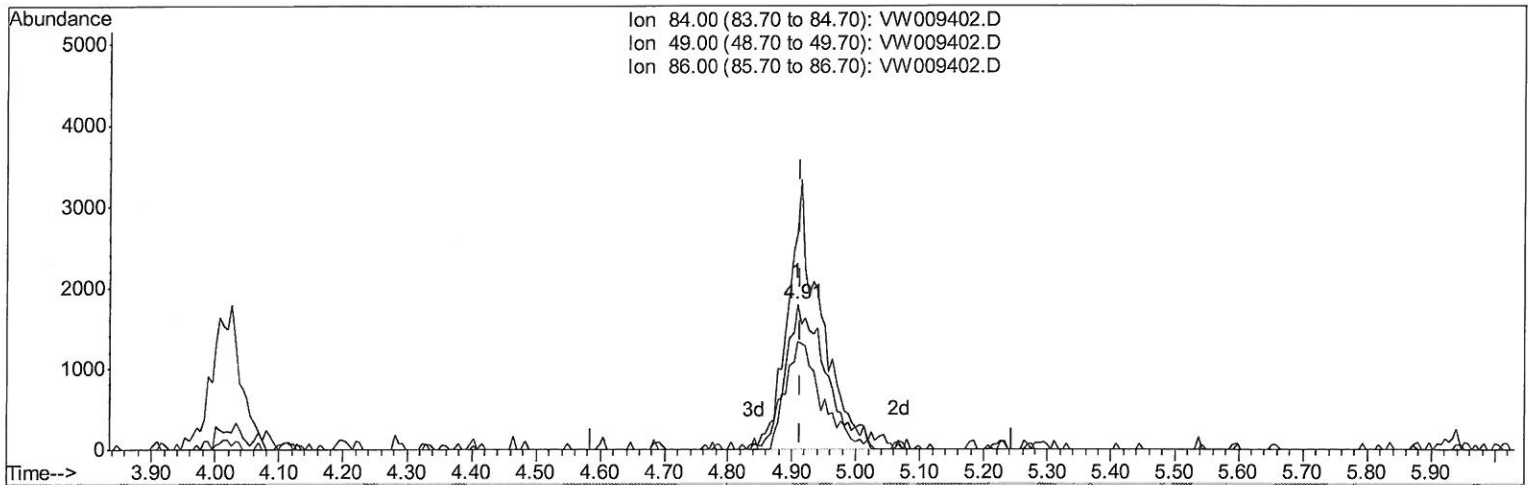

TIC: VW009402.D

(16) Methylene chloride (T)
4.909min (-0.006) 1.53ug/L m
response 7823

*7 mld
4/5/19*

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	149.13
86.00	63.50	74.54
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032319\
Quantitation Report (QT Reviewed)

Data File : VW009402.D
Acq On : 23 Mar 2019 21:11
Operator : SY/VA
Sample : K2062-18
Misc : 4.20G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF0H5

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:33:36 AM

Quant Time: Mar 24 00:31:38 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 23:52:05 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	349856	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	337899	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	153555	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	88082	21.07	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.28%
7) Chloroethane-d5	2.89	69	89462	18.29	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.16%
10) 1,1-Dichloroethene-d2	4.01	63	140362	15.53	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.12%
20) 2-Butanone-d5	7.07	46	86588	50.08	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.16%
24) Chloroform-d	7.65	84	217429	22.77	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.08%
26) 1,2-Dichloroethane-d4	8.30	65	135048	23.48	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.92%
29) Benzene-d6	8.27	84	386429	20.74	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.96%
33) 1,2-Dichloropropane-d6	9.27	67	121545	21.72	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.88%
37) Toluene-d8	10.32	98	334484	19.41	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.64%
38) trans-1,3-Dichloropropene-	10.58	79	54271	19.31	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.24%
39) 2-Hexanone-d5	10.93	63	63881	47.12	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.24%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	134012	24.31	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.24%
61) 1,2-Dichlorobenzene-d4	13.85	152	139067	23.62	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.48%

Target Compounds

					Qvalue
16) Methylene chloride	4.91	84	7823m	1.533	ug/L
47) Tetrachloroethene	10.86	164	26606	6.390	ug/L

7MO
4/5/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed