

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032319\
Quantitation Report (QT Reviewed)


Data File : VW009408.D
Acq On : 23 Mar 2019 23:54
Operator : SY/VA
Sample : K2083-02
Misc : 4.92G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
BF0N0

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:33:42 AM

Quant Time: Mar 24 01:02:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 23:52:05 2019
Response via : Initial Calibration

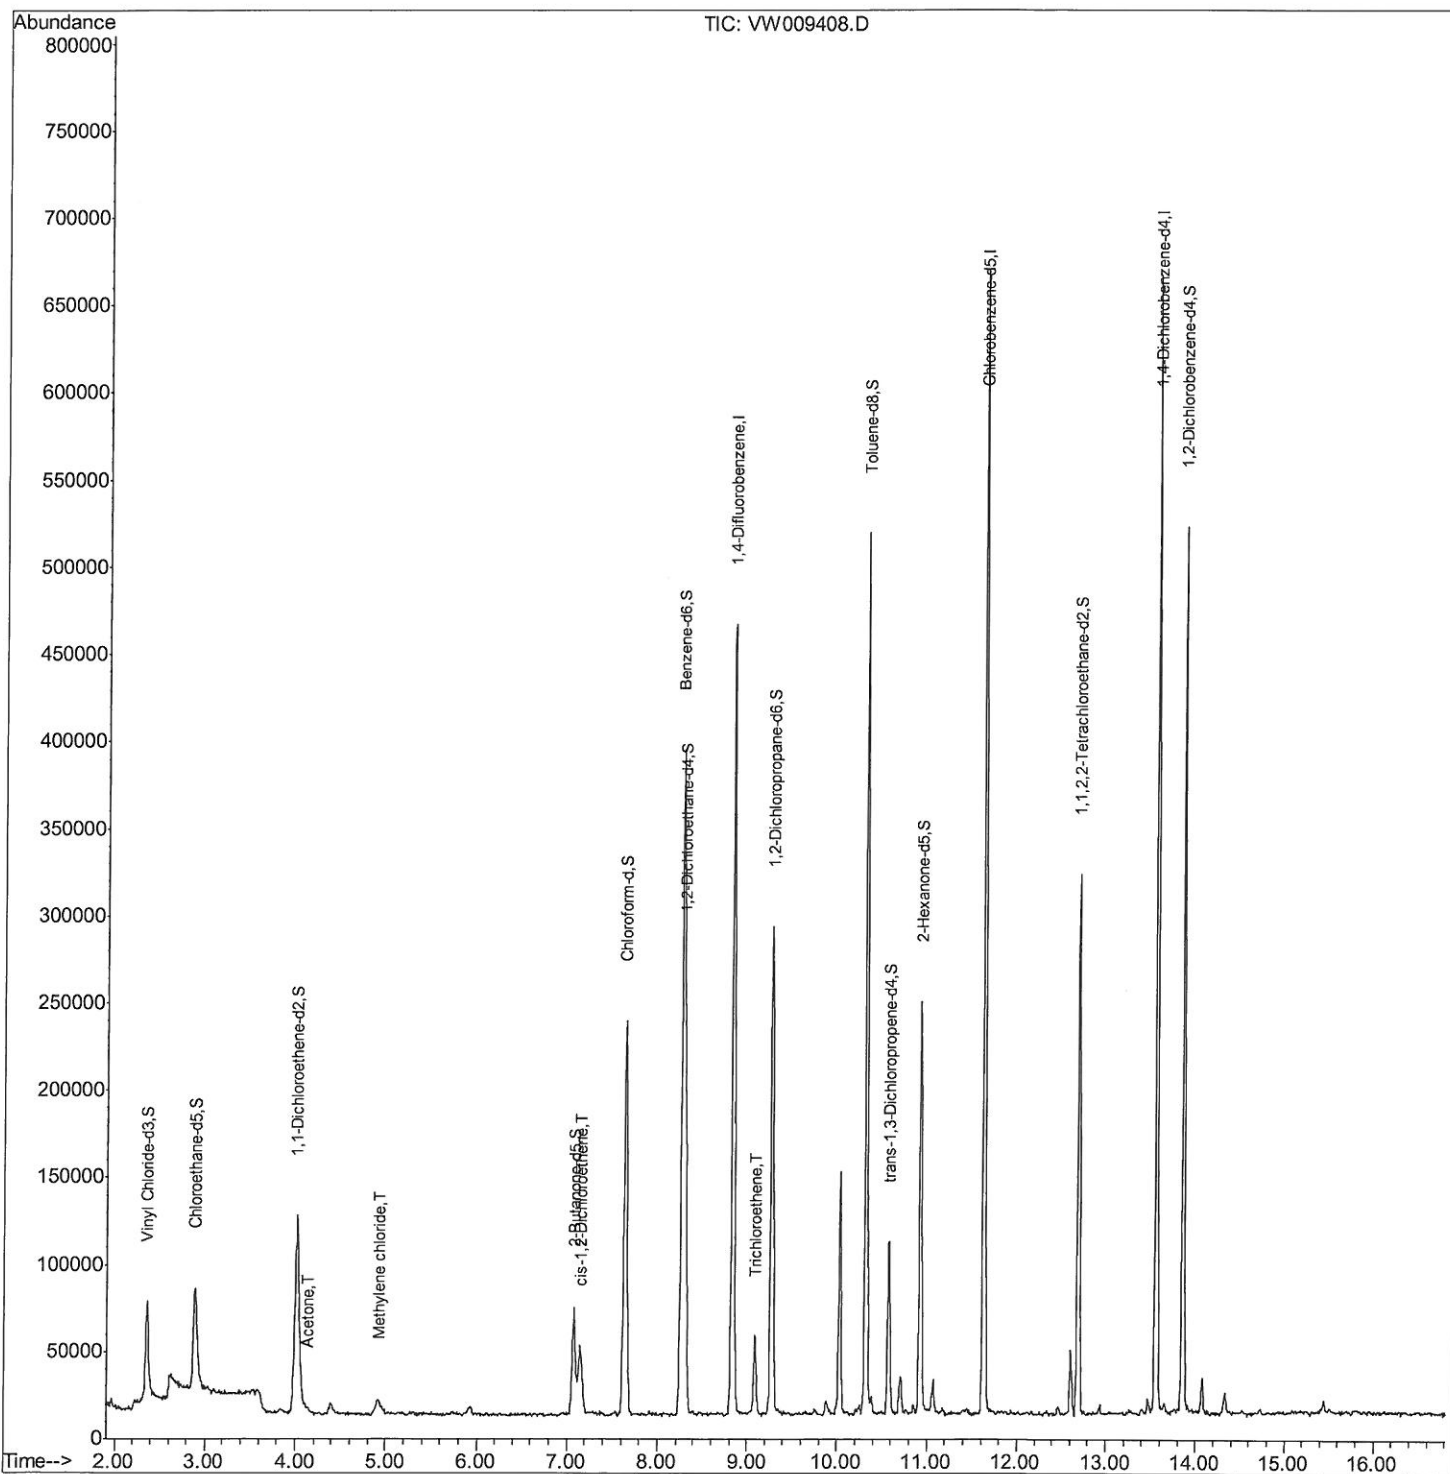

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032319\
Quantitation Report (Qedit)




Data File : VW009408.D
Acq On : 23 Mar 2019 23:54
Operator : SY/VA
Sample : K2083-02
Misc : 4.92G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF0N0

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:33:42 AM

Quant Time: Mar 24 01:00:51 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 23:52:05 2019
Response via : Initial Calibration

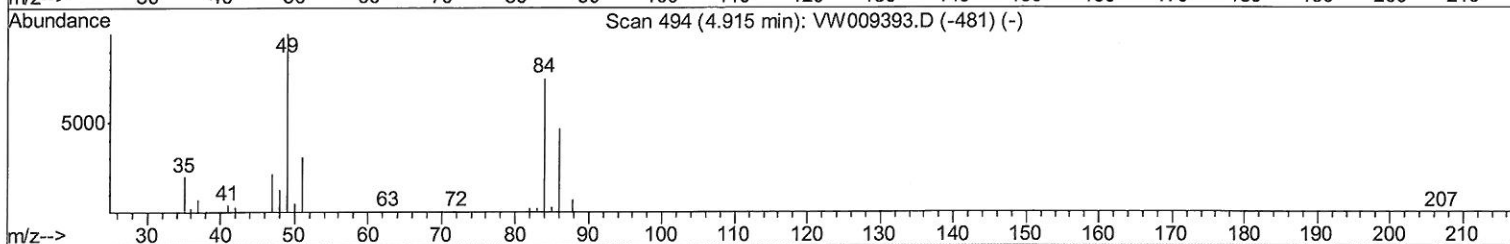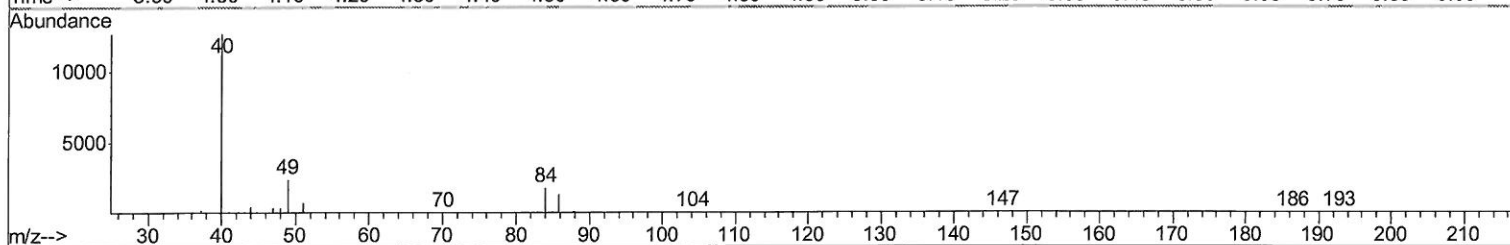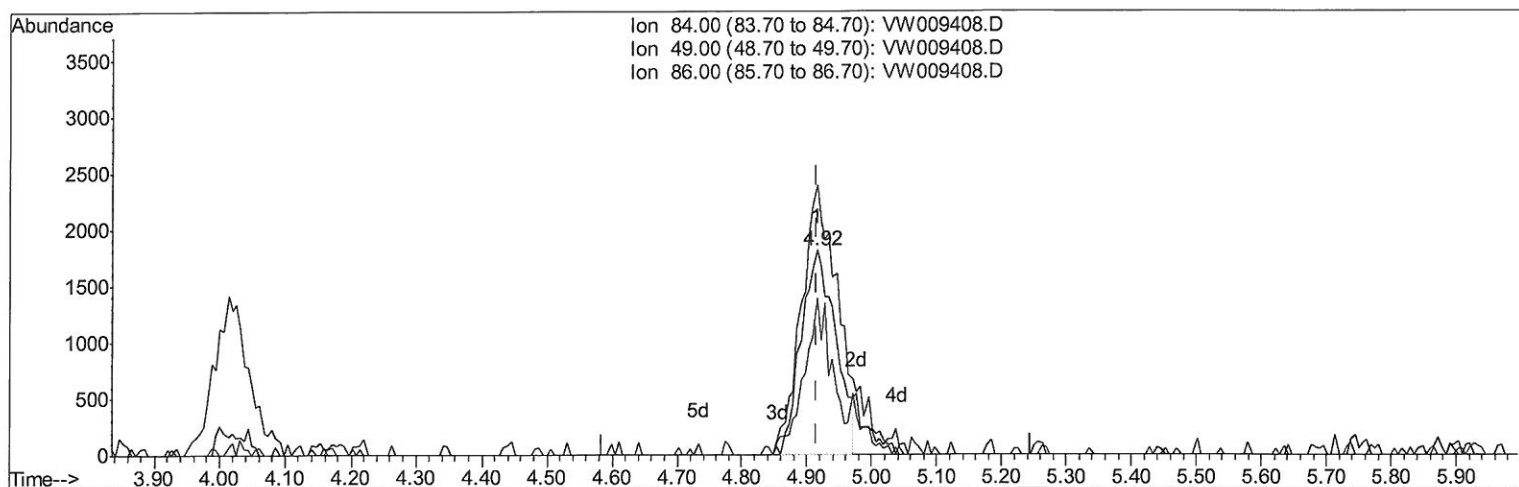

TIC: VW009408.D

(16) Methylene chloride (T)

4.915min (-0.000) 1.29ug/L

response 6693

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	131.94
86.00	63.50	76.56
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032319\
Quantitation Report (Qedit)




Data File : VW009408.D
Acq On : 23 Mar 2019 23:54
Operator : SY/VA
Sample : K2083-02
Misc : 4.92G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF0N0

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:33:42 AM

Quant Time: Mar 24 01:00:51 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 23:52:05 2019
Response via : Initial Calibration

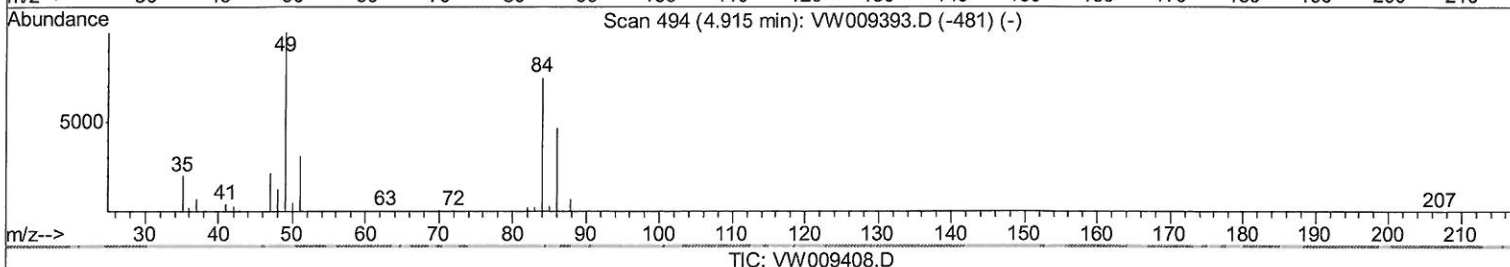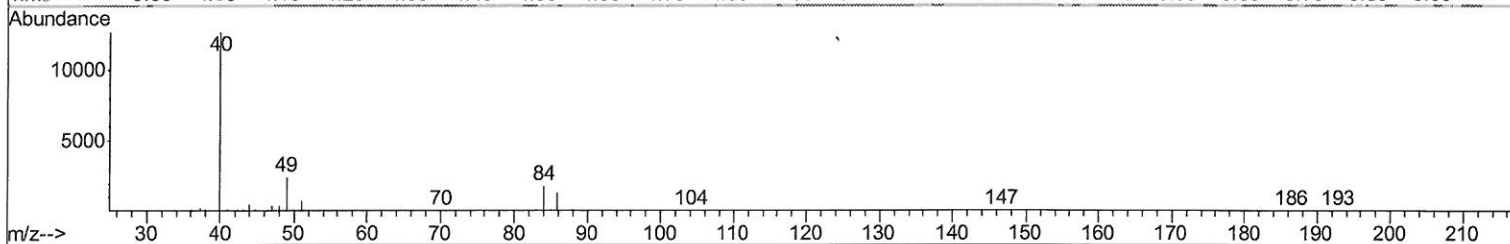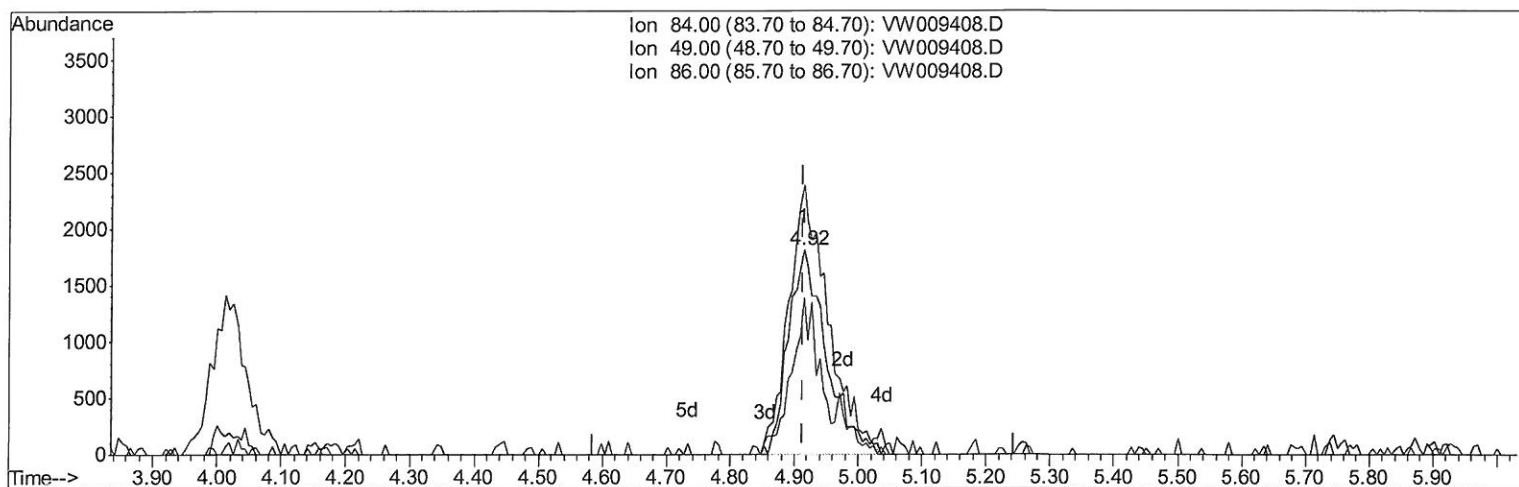

TIC: VW009408.D

(16) Methylene chloride (T)

4.915min (-0.000) 1.44ug/L m

response 7463

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	131.94
86.00	63.50	76.56
0.00	0.00	0.00

7 MLO
4/5/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032319\
Quantitation Report (QT Reviewed)

Data File : VW009408.D
Acq On : 23 Mar 2019 23:54
Operator : SY/VA
Sample : K2083-02
Misc : 4.92G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF0N0

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:33:42 AM

Quant Time: Mar 24 01:02:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 23:52:05 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	356006	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	344982	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	156700	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	80902	19.02	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.08%
7) Chloroethane-d5	2.89	69	85595	17.19	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.76%
10) 1,1-Dichloroethene-d2	4.02	63	131700	14.32	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.28%
20) 2-Butanone-d5	7.07	46	96372	54.78	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.56%
24) Chloroform-d	7.64	84	204302	21.03	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.12%
26) 1,2-Dichloroethane-d4	8.30	65	128537	21.96	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.84%
29) Benzene-d6	8.27	84	365371	19.20	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	76.80%
33) 1,2-Dichloropropane-d6	9.27	67	117320	20.53	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	82.12%
37) Toluene-d8	10.32	98	316559	17.99	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	71.96%
38) trans-1,3-Dichloropropene-	10.58	79	49107	17.11	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	68.44%
39) 2-Hexanone-d5	10.93	63	69020	49.87	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.74%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	135001	23.99	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.96%
61) 1,2-Dichlorobenzene-d4	13.86	152	126353	21.03	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.12%

Target Compounds

					Qvalue	
13) Acetone	4.12	43	4151	2.877	ug/L	51
16) Methylene chloride	4.92	84	7463m	1.438	ug/L	94
22) cis-1,2-Dichloroethene	7.16	96	7451	1.492	ug/L	94
35) Trichloroethene	9.09	95	14205	2.823	ug/L	98

7 MQ
4/5/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed