

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032319\
Quantitation Report (QT Reviewed)


Data File : VW009409.D
Acq On : 24 Mar 2019 00:22
Operator : SY/VA
Sample : K2083-03
Misc : 5.50G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF0N1

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:33:42 AM

Quant Time: Mar 24 01:04:33 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 23:52:05 2019
Response via : Initial Calibration

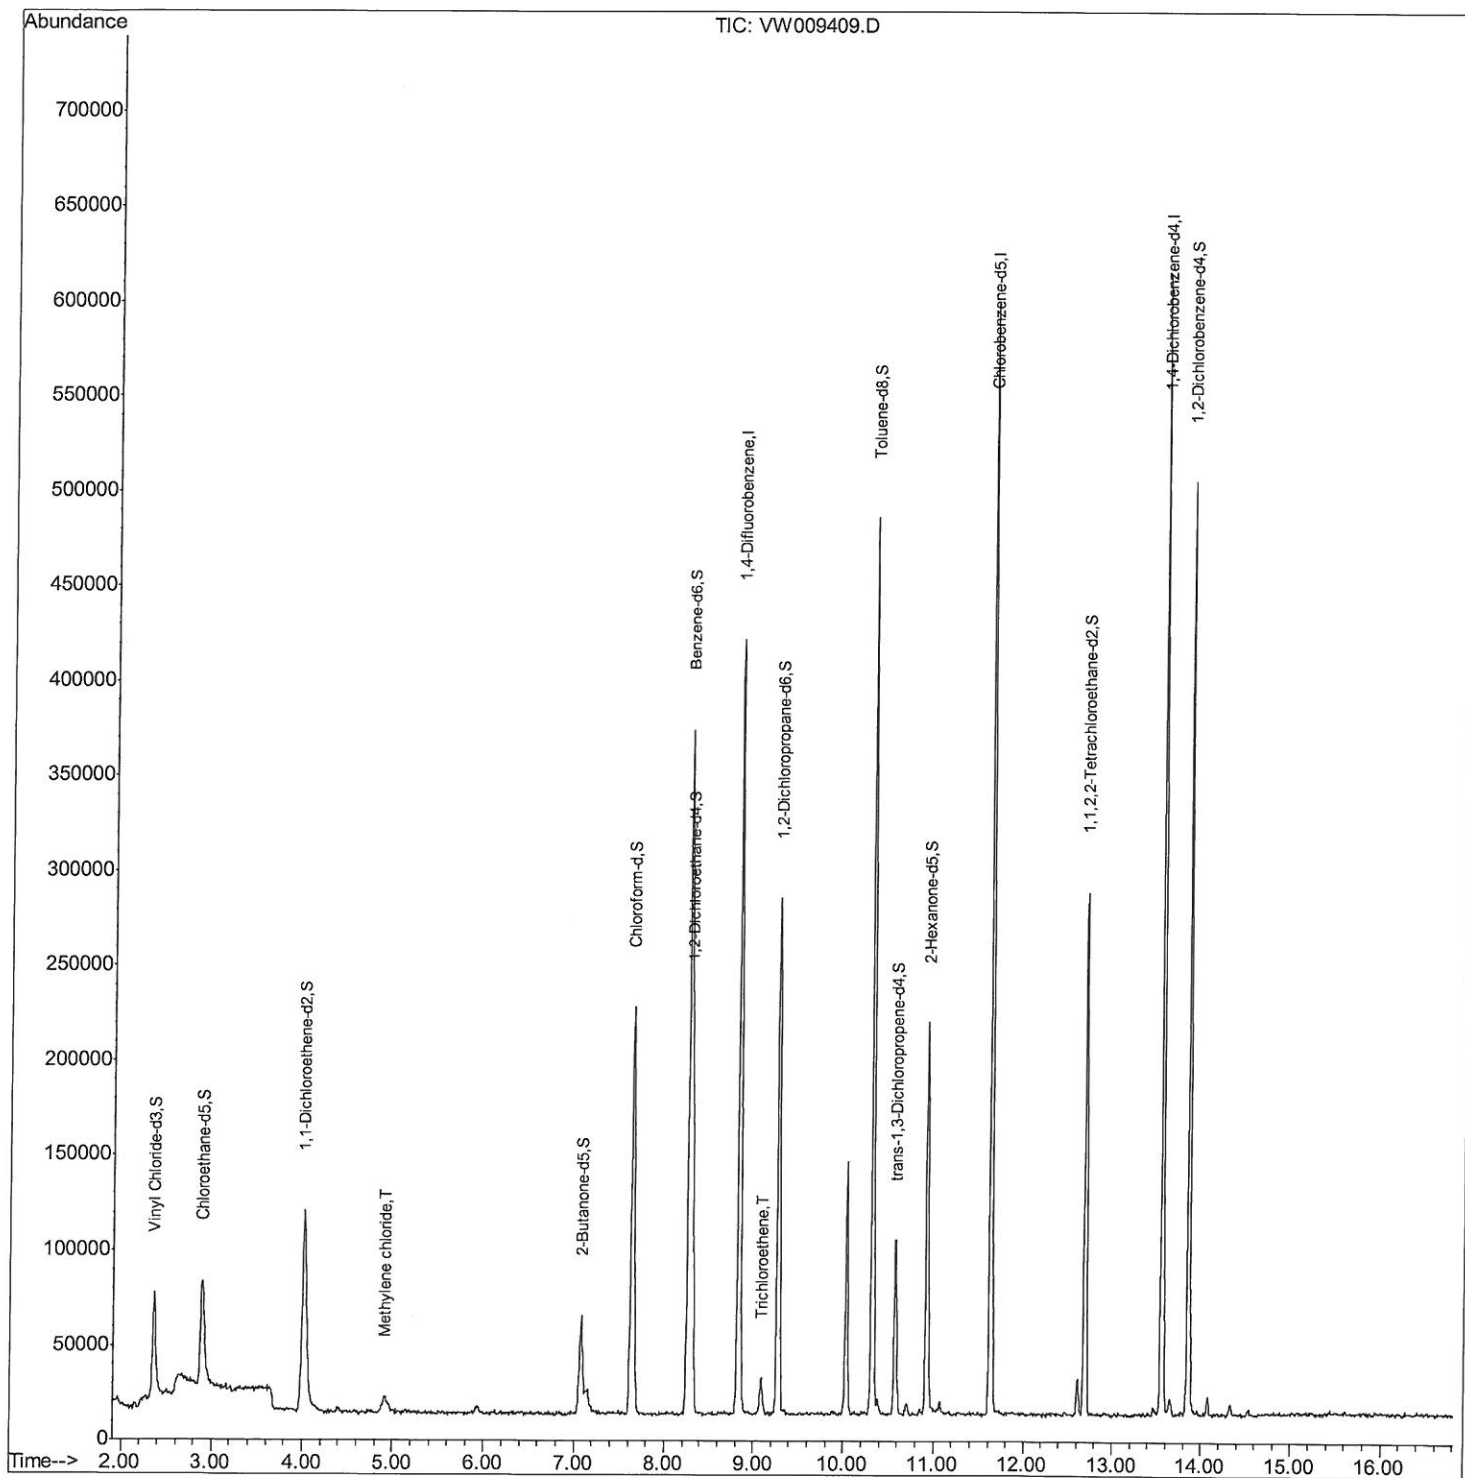

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032319\
Quantitation Report (Qedit)




Data File : VW009409.D
Acq On : 24 Mar 2019 00:22
Operator : SY/VA
Sample : K2083-03
Misc : 5.50G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF0N1

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:33:42 AM

Quant Time: Mar 24 00:56:07 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 23:52:05 2019
Response via : Initial Calibration

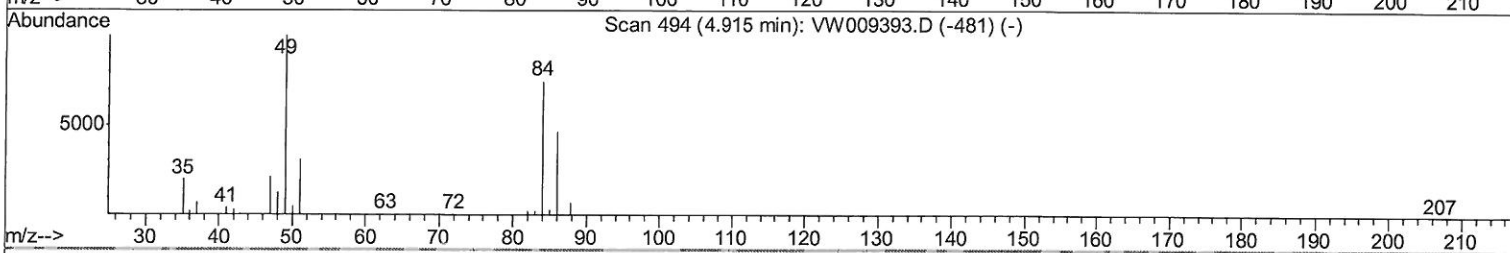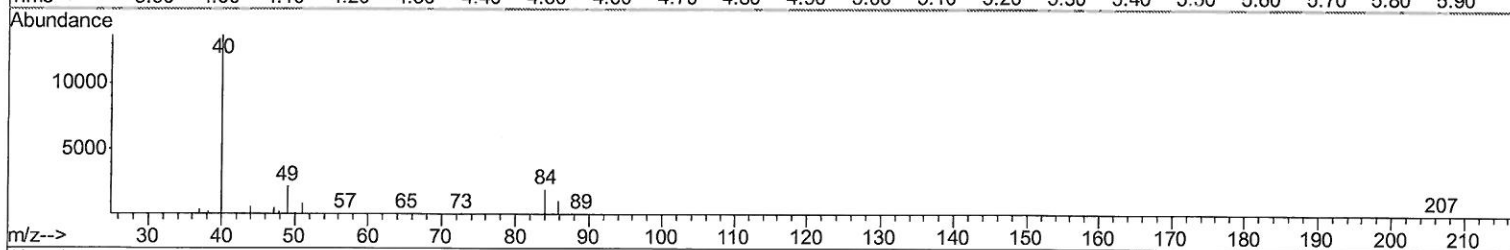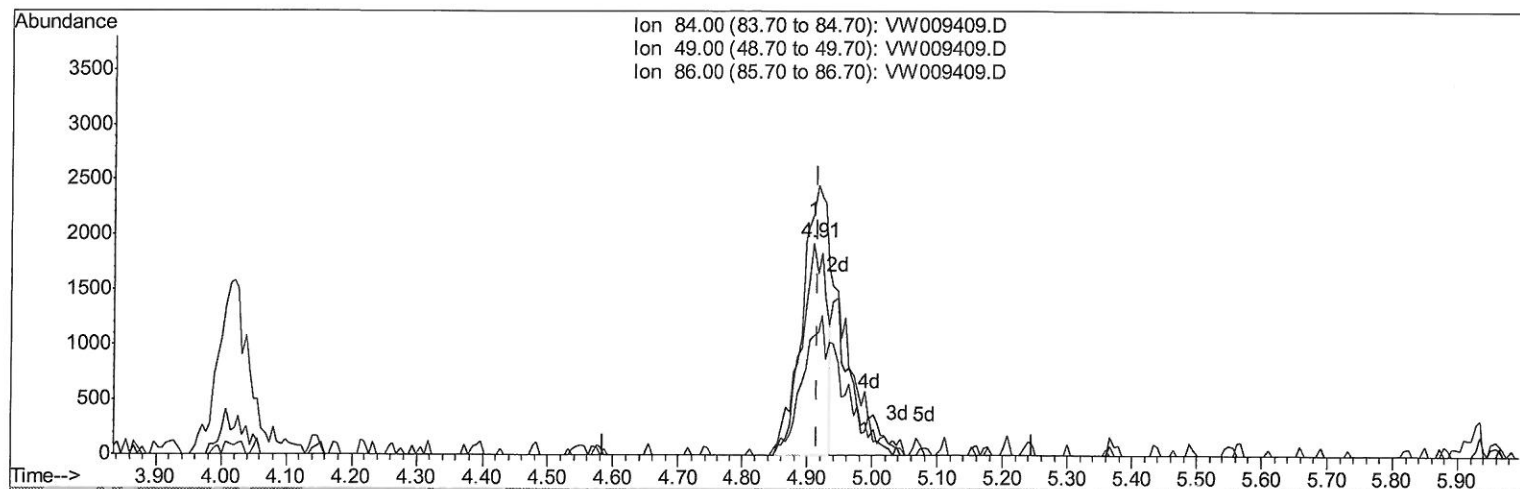

TIC: VW009409.D

(16) Methylene chloride (T)

4.909min (-0.006) 1.12ug/L

response 5172

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	113.12
86.00	63.50	55.76
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032319\
Quantitation Report (Qedit)




Data File : VW009409.D
Acq On : 24 Mar 2019 00:22
Operator : SY/VA
Sample : K2083-03
Misc : 5.50G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF0N1

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:33:42 AM

Quant Time: Mar 24 00:56:07 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 23:52:05 2019
Response via : Initial Calibration

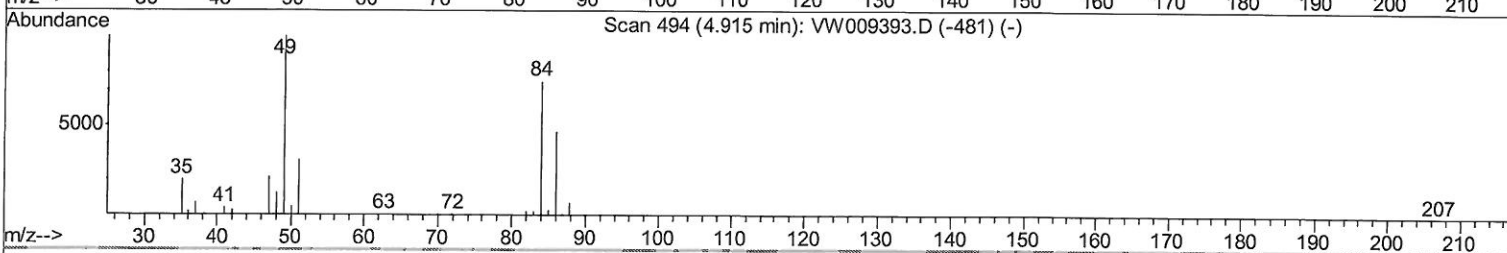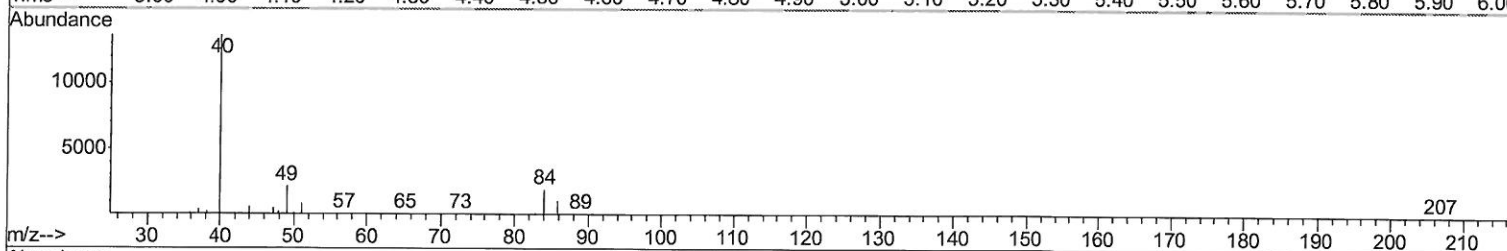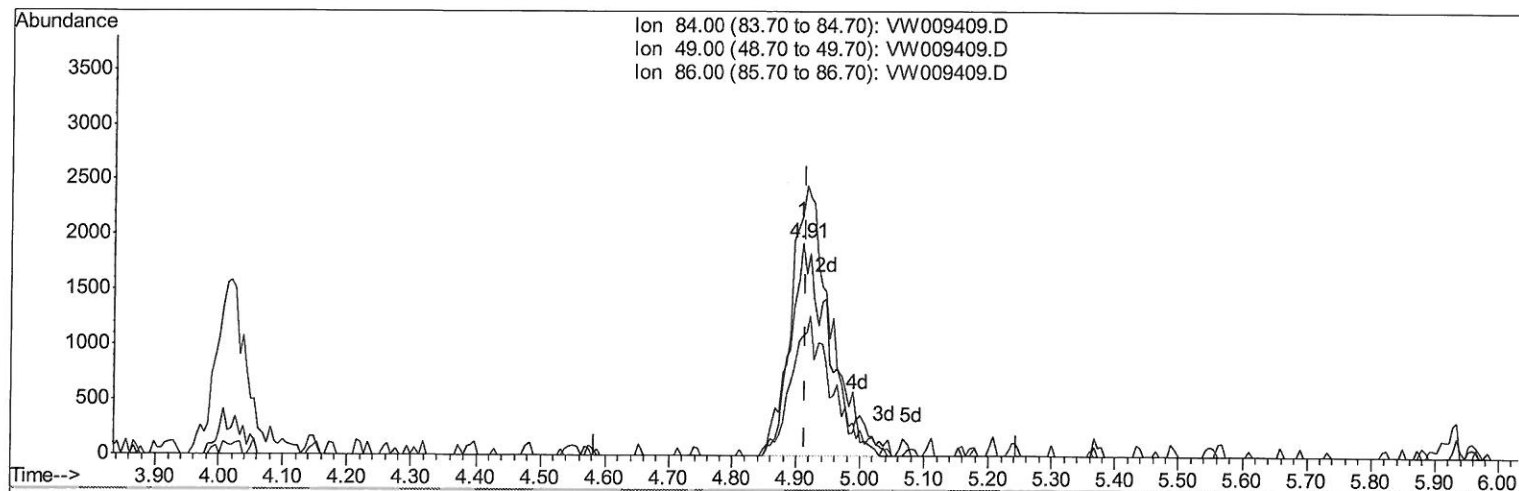

TIC: VW009409.D

(16) Methylene chloride (T)

4.909min (-0.006) 1.72ug/L m

response 7926

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	113.12
86.00	63.50	55.76
0.00	0.00	0.00

MO
4/5/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032319\
Quantitation Report (QT Reviewed)

Data File : VW009409.D
Acq On : 24 Mar 2019 00:22
Operator : SY/VA
Sample : K2083-03
Misc : 5.50G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF0N1

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:33:42 AM

Quant Time: Mar 24 01:04:33 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 23:52:05 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	316812	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	314255	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	142443	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	82384	21.76	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.04%
7) Chloroethane-d5	2.89	69	83090	18.76	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.04%
10) 1,1-Dichloroethene-d2	4.01	63	130472	15.95	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.80%
20) 2-Butanone-d5	7.08	46	82366	52.61	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.22%
24) Chloroform-d	7.64	84	193472	22.38	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.52%
26) 1,2-Dichloroethane-d4	8.31	65	120758	23.19	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.76%
29) Benzene-d6	8.27	84	349184	20.15	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	80.60%
33) 1,2-Dichloropropane-d6	9.27	67	112526	21.62	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.48%
37) Toluene-d8	10.32	98	300825	18.77	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	75.08%
38) trans-1,3-Dichloropropene-	10.58	79	47124	18.03	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	72.12%
39) 2-Hexanone-d5	10.93	63	59642	47.31	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.62%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	124974	24.38	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.52%
61) 1,2-Dichlorobenzene-d4	13.86	152	126762	23.21	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.84%

Target Compounds

16) Methylene chloride	4.91	84	7926m	1.716	ug/L	Qvalue
35) Trichloroethene	9.09	95	5643	1.231	ug/L	95

7 M8
4/5/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed