

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032319\
 Data File : VW009389.D
 Acq On : 23 Mar 2019 14:39
 Operator : SY/VA
 Sample : K2062-01
 Misc : 5.88G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF0G8

Manual Integrations
 APPROVED

MMDadoda
 3/25/2019 8:33:28 AM

Quant Time: Mar 23 23:34:21 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 23 22:42:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	360003	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	351091	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	158194	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	89198	20.73	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.92%
7) Chloroethane-d5	2.89	69	93055	18.49	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.96%
10) 1,1-Dichloroethene-d2	4.01	63	142208	15.29	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.16%
20) 2-Butanone-d5	7.07	46	79080	44.45	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.90%
24) Chloroform-d	7.65	84	222115	22.61	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.44%
26) 1,2-Dichloroethane-d4	8.30	65	135709	22.93	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.72%
29) Benzene-d6	8.27	84	390333	20.16	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	80.64%
33) 1,2-Dichloropropane-d6	9.27	67	126961	21.83	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.32%
37) Toluene-d8	10.32	98	345887	19.32	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.28%
38) trans-1,3-Dichloropropene-	10.58	79	55959	19.16	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.64%
39) 2-Hexanone-d5	10.93	63	56305	39.98	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.96%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	124580	21.75	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.00%
61) 1,2-Dichlorobenzene-d4	13.86	152	138004	22.75	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.00%

Target Compounds				Ovalue
16) Methylene chloride	4.93	84	13778m	2.624 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW032319\
Data File : VW009389.D
Acq On : 23 Mar 2019 14:39
Operator : SY/VA
Sample : K2062-01
Misc : 5.88G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BF0G8

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:33:28 AM

Quant Time: Mar 23 23:34:21 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 22:42:53 2019
Response via : Initial Calibration

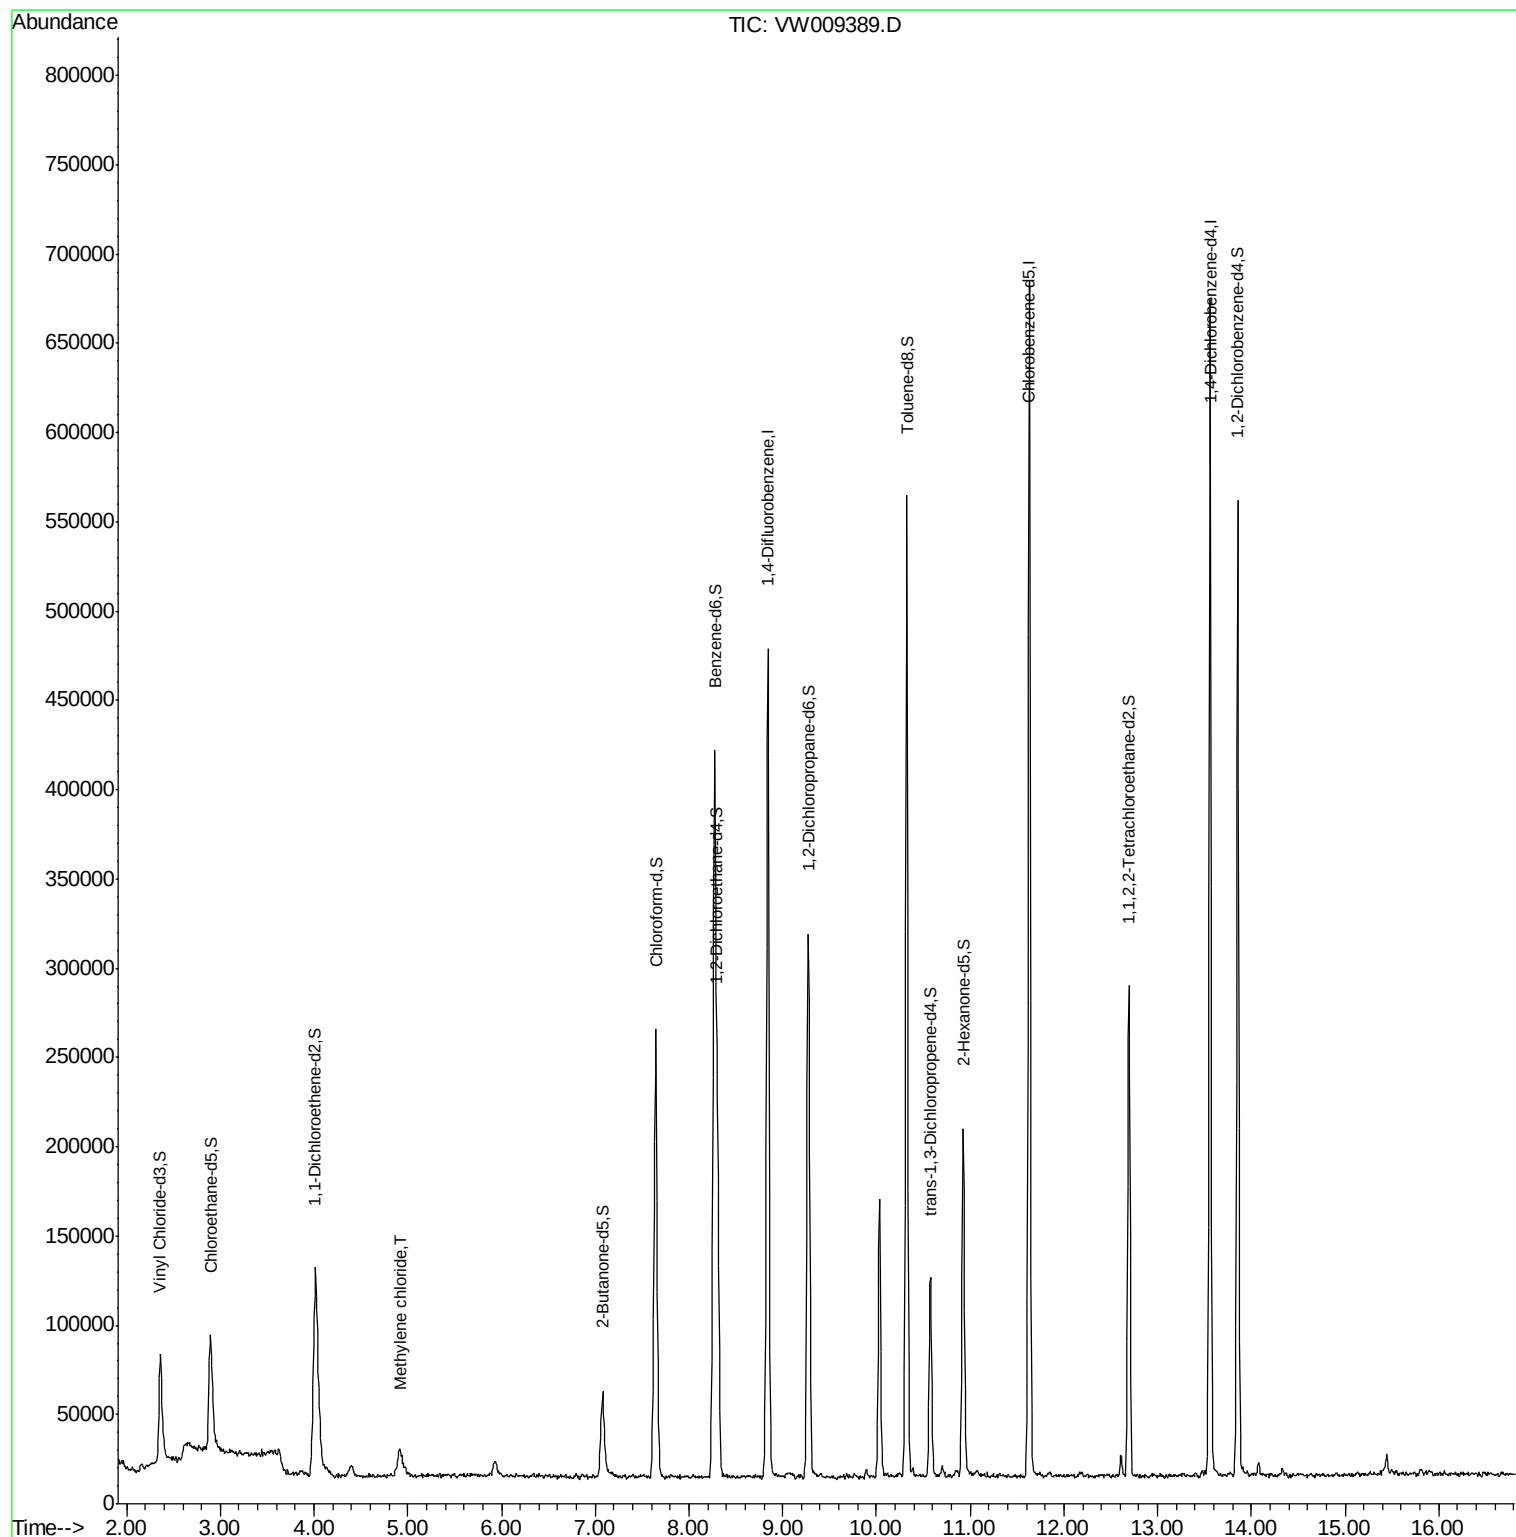

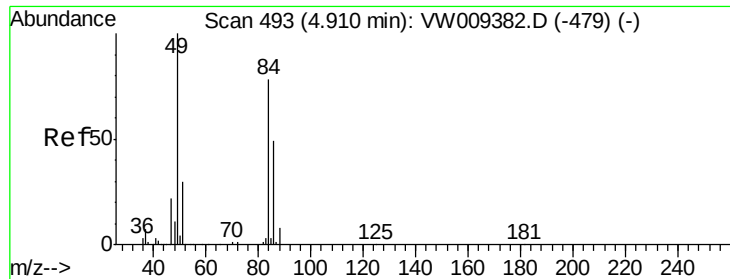

#16
 Methvlene chloride
 Concen: 2.624 ug/L m
 RT: 4.93 min Scan# 496
 Delta R.T. 0.02 min
 Lab File: VW009389.D
 Acq: 23 Mar 2019 14:39

Instrument :
 MSVOA_W
 ClientSampleId :
 BF0G8

Tot Ion	Ratio	Lower	Upper
84	100		
49	119.6	96.0	178.2
86	57.0	44.4	82.5

Manual Integrations
 APPROVED

MMDadoda
 3/25/2019 8:33:28 AM

