


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032319\
 Data File : VW009381.D
 Acq On : 23 Mar 2019 09:37
 Operator : SY/VA
 Sample : BFB08
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB08

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Title : VOC Analysis
 Last Update : Sat Mar 23 23:52:05 2019

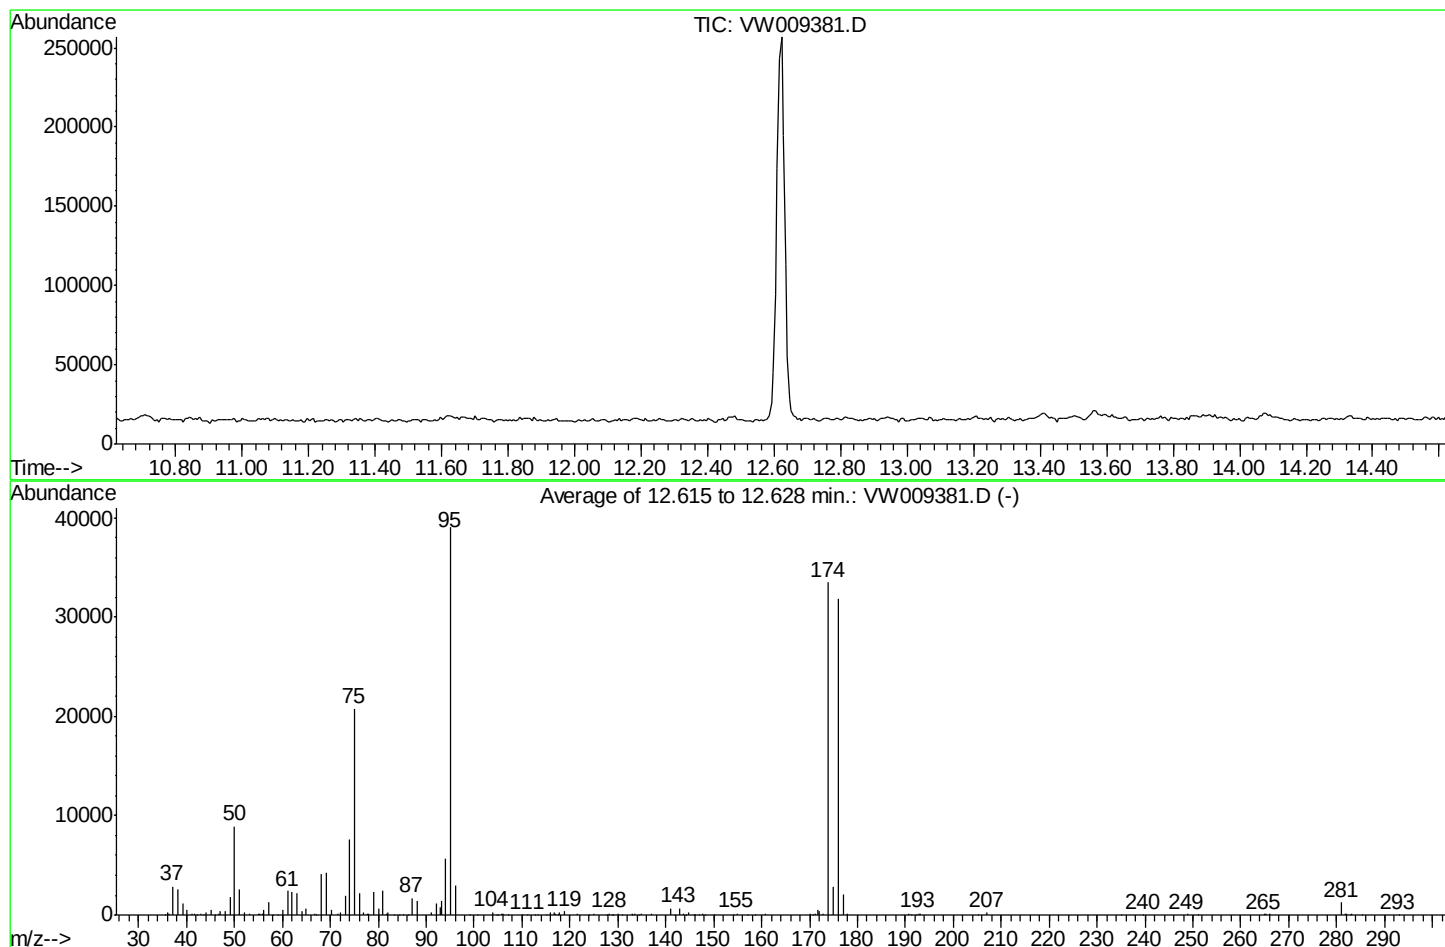

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	8950	PASS
75	95	30	80	53.2	20757	PASS
95	95	100	100	100.0	39040	PASS
96	95	5	9	7.5	2923	PASS
173	174	0.00	2	0.5	163	PASS
174	95	50	120	85.8	33477	PASS
175	174	5	9	8.5	2850	PASS
176	174	95	101	95.3	31896	PASS
177	176	5	9	6.4	2051	PASS

Scan 1749 (12.567 min): VW009381.D
BFB08

m/z	Abundance
35.90	139.0
36.70	70.0
40.00	13465.0
43.20	79.0
44.00	403.0
48.10	63.0
55.70	63.0
56.70	66.0
58.80	68.0
59.50	57.0
64.50	52.0
66.10	69.0
131.10	55.0
139.80	65.0
279.70	73.0

Instrument :
MSVOA_W
ClientSampleId :
BFB08

m/z	Abundance
36.00	786.0
37.10	3450.0
38.00	2863.0
39.10	1457.0
40.00	14049.0
41.00	213.0
41.60	89.0
42.20	60.0
42.90	109.0
43.40	162.0
44.00	678.0
45.10	426.0
47.10	694.0
48.00	532.0
49.10	1981.0
50.00	9849.0
51.10	3222.0
51.90	258.0
53.20	86.0
55.00	82.0
55.90	713.0
57.10	1558.0
58.00	102.0
59.20	127.0
59.90	544.0
61.10	2614.0
62.00	2275.0
63.10	2214.0
64.10	288.0
65.00	605.0
66.80	143.0
68.00	4392.0
69.00	4532.0
70.10	338.0
71.60	123.0
72.10	235.0
73.00	2033.0
74.00	8430.0
75.00	21928.0
76.00	2428.0
77.00	295.0
77.90	158.0
78.90	3025.0
80.10	649.0
80.90	2500.0
81.80	574.0
87.10	1831.0
88.00	1841.0
91.00	293.0
92.00	1368.0
92.90	2198.0
94.10	5466.0
95.00	42584.0
96.00	3370.0
99.20	174.0
100.70	58.0
103.90	351.0
104.70	59.0
105.90	340.0
111.10	93.0
112.70	75.0
113.20	71.0
115.90	259.0
117.10	450.0
118.00	169.0
118.90	277.0
121.60	145.0
123.90	56.0
124.90	168.0
127.70	135.0
128.80	60.0
130.00	145.0
132.90	209.0
133.60	256.0
134.20	100.0
135.00	163.0
137.10	86.0
141.00	606.0
141.80	62.0
142.80	636.0
143.80	55.0
144.90	451.0
145.70	87.0
146.00	102.0
147.00	81.0
147.70	166.0
148.20	52.0
154.90	99.0
157.10	84.0
158.70	76.0
160.90	167.0
170.40	87.0

Instrument :
MSVOA_W
ClientSampleId :
BFB08

171.80	512.0
172.10	516.0
174.00	32680.0
175.00	2796.0
176.00	31160.0
176.90	1978.0
178.10	144.0
190.80	144.0
191.10	153.0
193.00	302.0
205.10	54.0
207.10	253.0
248.80	102.0
251.00	77.0
264.80	134.0
265.30	56.0
266.20	139.0
281.10	1843.0
281.90	370.0
282.90	169.0
292.90	53.0

Instrument :
MSVOA_W
ClientSampleId :
BFB08

m/z	Abundance
36.00	574.0
37.10	3171.0
38.10	2894.0
39.20	1210.0
40.00	14076.0
41.10	87.0
41.70	74.0
42.20	102.0
42.80	101.0
44.10	706.0
45.00	650.0
45.90	102.0
46.80	361.0
48.00	503.0
49.00	1838.0
50.10	10313.0
51.10	2917.0
52.00	371.0
53.10	253.0
55.20	212.0
56.10	853.0
57.10	1572.0
59.00	80.0
60.00	601.0
61.10	2772.0
62.10	2422.0
63.10	2657.0
64.10	457.0
65.00	768.0
66.70	100.0
68.00	4193.0
69.00	4575.0
70.10	849.0
71.70	234.0
73.10	2295.0
74.00	8611.0
75.00	23680.0
76.00	2665.0
76.90	288.0
77.60	249.0
79.00	2305.0
80.00	723.0
81.00	2562.0
82.00	541.0
83.20	75.0
84.30	60.0
86.20	106.0
86.90	1766.0
88.00	1533.0
90.90	193.0
92.00	1559.0
93.10	2540.0
94.10	6936.0
95.00	43448.0
96.10	3062.0
103.70	211.0
105.00	101.0
105.80	217.0
107.00	64.0
109.90	54.0
112.70	67.0
115.90	412.0
116.80	414.0
117.80	325.0
118.90	449.0
121.50	131.0
125.00	127.0
128.20	341.0
129.10	62.0
130.10	104.0
133.10	156.0
134.80	58.0
137.10	78.0
141.00	650.0
141.80	79.0
142.90	769.0
143.70	103.0
144.70	218.0
146.00	95.0
147.00	57.0
147.60	123.0
148.20	54.0
150.20	56.0
154.80	196.0
157.00	72.0
158.60	131.0
160.90	67.0
170.20	97.0
170.70	91.0
171.30	152.0
171.90	1009.0
173.90	36952.0

Instrument :
MSVOA_W
ClientSampleId :
BFB08

175.00	3429.0
176.00	35008.0
176.90	2585.0
178.00	172.0
190.60	81.0
190.90	65.0
192.20	63.0
192.70	254.0
205.20	72.0
207.10	168.0
235.10	68.0
248.90	125.0
264.90	187.0
266.10	120.0
279.60	85.0
281.00	1297.0
282.10	310.0
283.10	375.0
285.10	111.0
293.00	76.0

Instrument :
MSVOA_W
ClientSampleId :
BFB08

m/z	Abundance
35.40	112.0
36.20	435.0
37.10	1958.0
38.10	2103.0
39.00	984.0
40.00	13771.0
41.50	83.0
43.10	113.0
44.10	609.0
45.10	459.0
45.80	73.0
47.10	471.0
48.00	254.0
49.00	1503.0
50.10	6690.0
51.00	1677.0
52.00	99.0
53.20	170.0
55.00	214.0
56.10	796.0
57.10	844.0
60.00	478.0
61.00	1787.0
62.00	2160.0
63.10	1707.0
64.10	270.0
65.00	535.0
67.10	105.0
68.00	3750.0
69.10	3574.0
69.90	164.0
70.20	247.0
72.10	371.0
73.00	1377.0
74.00	5857.0
75.00	16664.0
76.00	1645.0
76.80	179.0
77.90	115.0
78.90	1510.0
79.90	421.0
80.90	2360.0
81.90	321.0
83.20	50.0
85.10	52.0
86.10	74.0
87.10	1639.0
88.00	1063.0
90.90	241.0
91.90	688.0
93.10	1792.0
94.00	4749.0
95.00	31088.0
96.00	2339.0
103.80	239.0
105.10	95.0
106.10	368.0
107.00	76.0
109.90	61.0
115.00	78.0
115.80	253.0
116.80	359.0
117.60	145.0
118.00	144.0
118.80	355.0
124.90	124.0
128.20	118.0
129.10	75.0
129.90	70.0
130.80	62.0
132.90	108.0
134.80	132.0
137.10	116.0
140.80	645.0
141.60	65.0
142.90	613.0
143.70	114.0
144.10	108.0
144.80	178.0
154.00	58.0
155.00	98.0
170.20	67.0
171.20	112.0
172.10	582.0
172.80	490.0
174.00	30800.0
174.90	2326.0
176.00	29520.0
177.00	1591.0
177.90	112.0
192.80	149.0
207.10	231.0

Instrument :
MSVOA_W
ClientSampleId :
BFB08

239.70	108.0
265.10	173.0
281.10	592.0
282.00	84.0
283.20	169.0
285.20	58.0

Instrument :
MSVOA_W
ClientSampleId :
BFB08