




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032524\
 Data File : VW028241.D
 Acq On : 25 Mar 2024 11:26
 Operator : SY/MD
 Sample : P1839-11
 Misc : 3.54g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOLY9

Manual IntegrationsAPPROVED

Quant Time: Mar 26 01:18:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 26 01:17:39 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/26/2024
 Supervised By :Mahesh Dadoda 03/26/2024

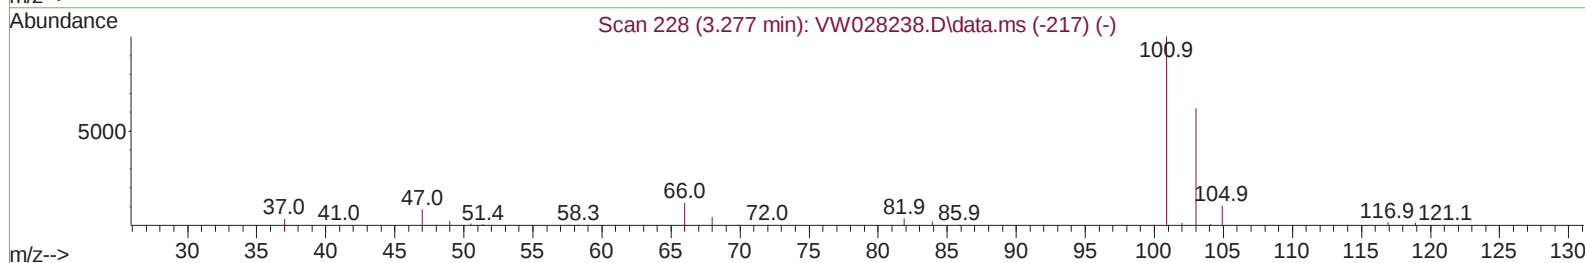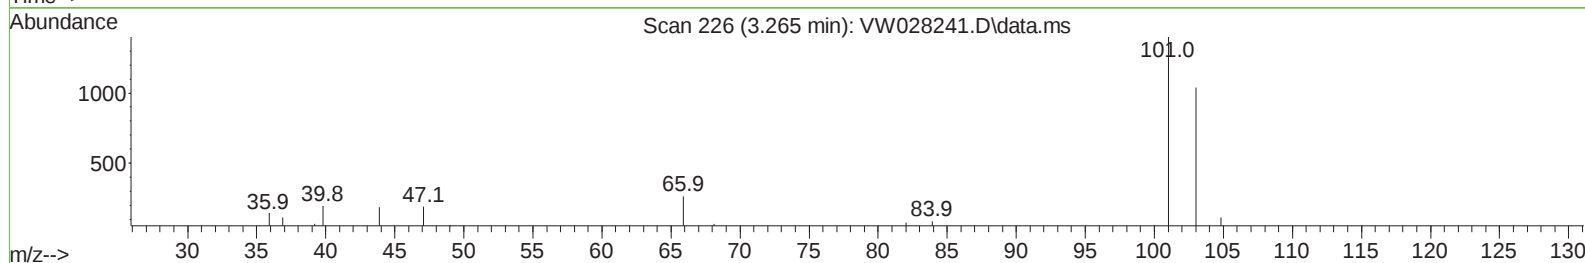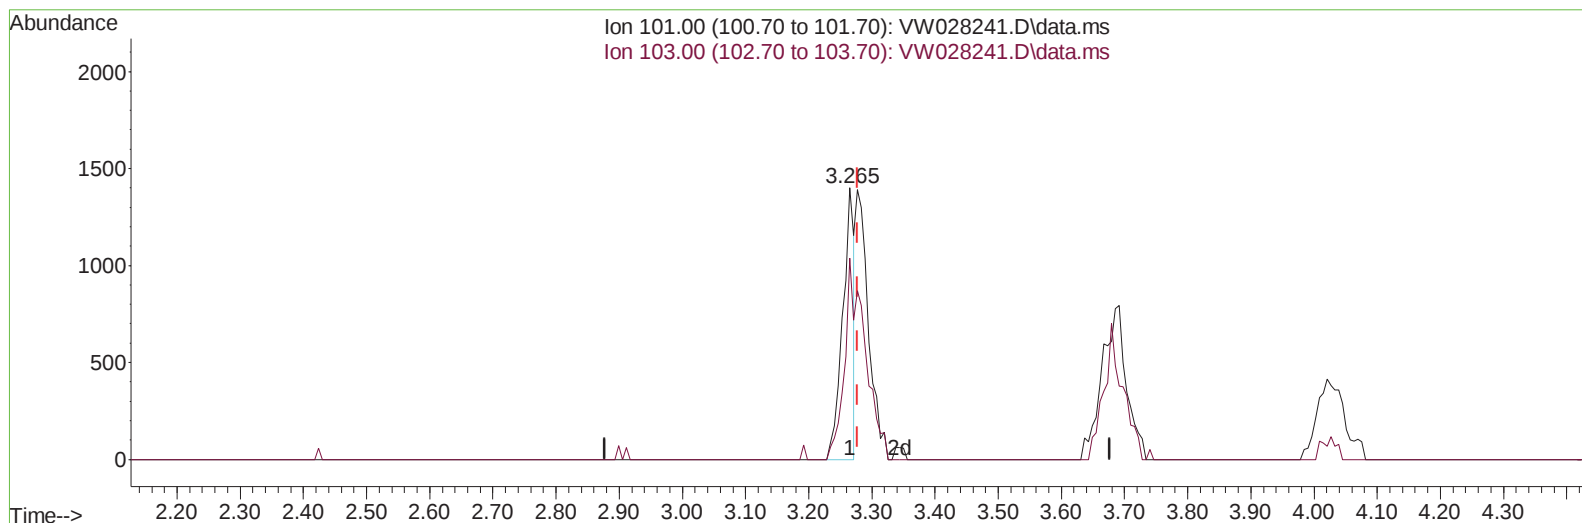

TIC: VW028241.D\data.ms

(9) Trichlorofluoromethane (T)

3.265min (-0.012) 0.38 ug/L

response 1776

Ion	Exp%	Act%
101.00	100.00	100.00
103.00	63.60	61.60
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032524\
 Data File : VW028241.D
 Acq On : 25 Mar 2024 11:26
 Operator : SY/MD
 Sample : P1839-11
 Misc : 3.54g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOLY9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/26/2024
 Supervised By :Mahesh Dadoda 03/26/2024

Quant Time: Mar 26 01:18:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 26 01:17:39 2024
 Response via : Initial Calibration

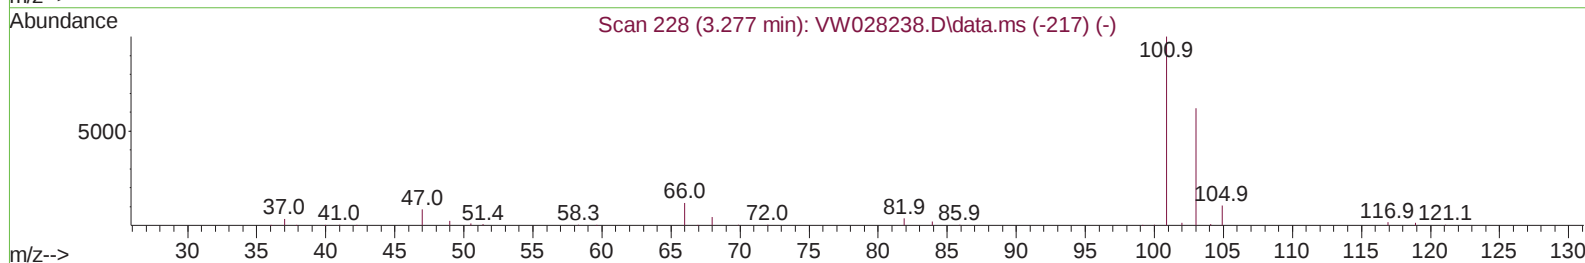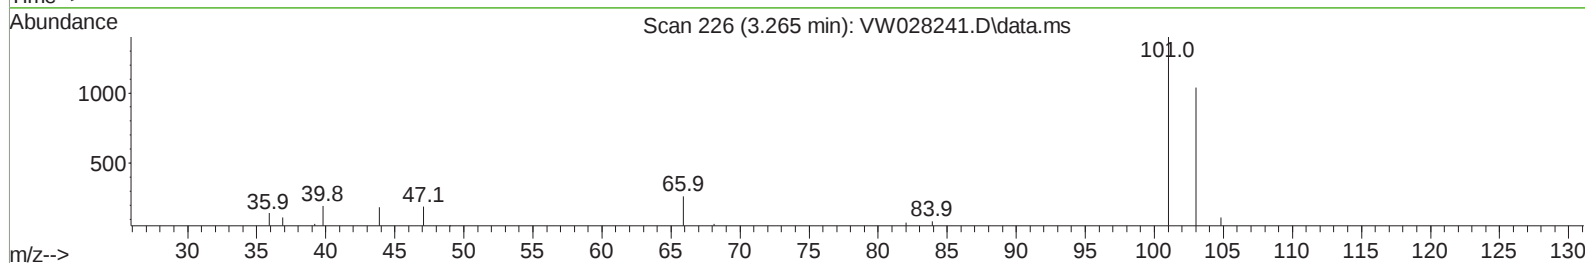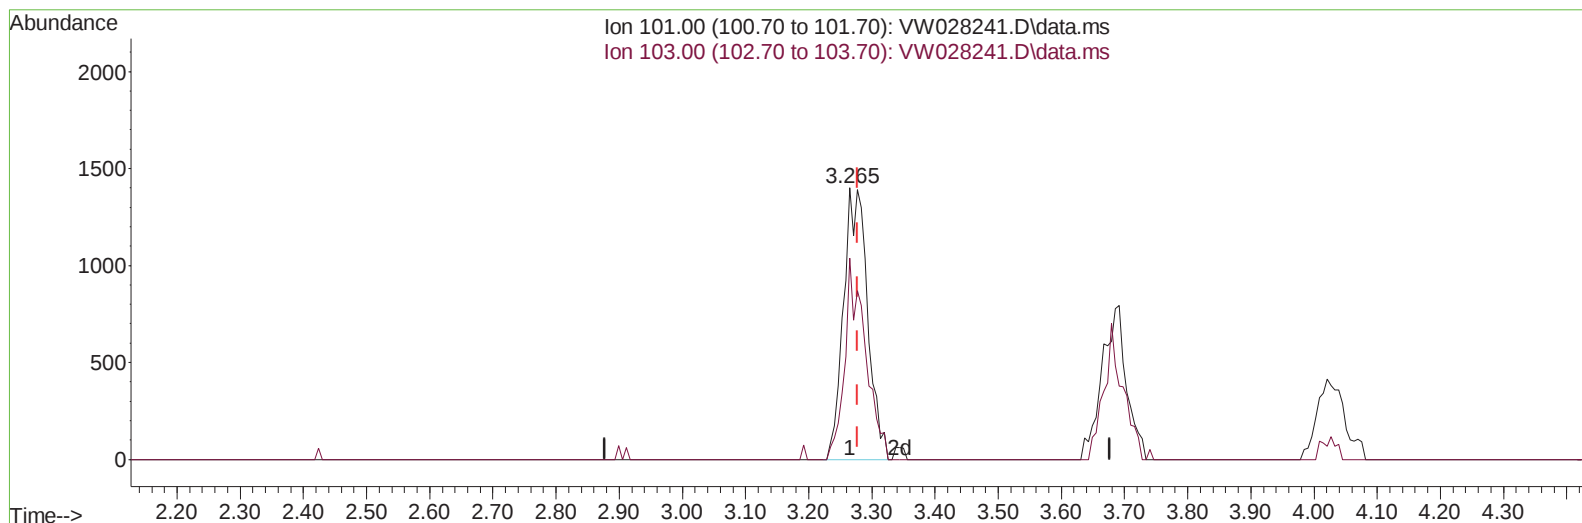

TIC: VW028241.D\data.ms

(9) Trichlorofluoromethane (T)

3.265min (-0.012) 0.79 ug/L m

response 3711

Ion	Exp%	Act%
101.00	100.00	100.00
103.00	63.60	29.48#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032524\
 Data File : VW028241.D
 Acq On : 25 Mar 2024 11:26
 Operator : SY/MD
 Sample : P1839-11
 Misc : 3.54g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E0LY9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/26/2024
 Supervised By :Mahesh Dadoda 03/26/2024

Quant Time: Mar 26 01:18:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 26 01:17:39 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		334408	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		219494	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		58556	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		63908	16.333	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	65.320%		
7) Chloroethane-d5	2.899	69		48509	17.745	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	71.000%		
11) 1,1-Dichloroethene-d2	4.027	65		42046	16.946	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	67.800%		
21) 2-Butanone-d5	7.081	46		35546	30.802	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	61.600%		
24) Chloroform-d	7.654	84		180275	18.282	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	73.120%		
26) 1,2-Dichloroethane-d4	8.307	65		96053	17.676	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	70.720%		
32) Benzene-d6	8.276	84		345192	25.759	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	103.040%		
36) 1,2-Dichloropropane-d6	9.270	67		99643	25.838	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	103.360%		
41) Toluene-d8	10.325	98		274575	22.214	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	88.840%		
43) trans-1,3-Dichloroprop...	10.575	79		36273	20.709	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	82.840%		
47) 2-Hexanone-d5	10.922	63		25197	39.527	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	79.060%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		47045	16.514	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	66.040%		
66) 1,2-Dichlorobenzene-d4	13.848	152		41035	19.237	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	76.960%		
Target Compounds							Qvalue
9) Trichlorofluoromethane	3.265	101		3711m	0.789	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032524\
Data File : VW028241.D
Acq On : 25 Mar 2024 11:26
Operator : SY/MD
Sample : P1839-11
Misc : 3.54g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E0LY9

Manual IntegrationsAPPROVED

Quant Time: Mar 26 01:18:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 26 01:17:39 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/26/2024
Supervised By :Mahesh Dadoda 03/26/2024

