
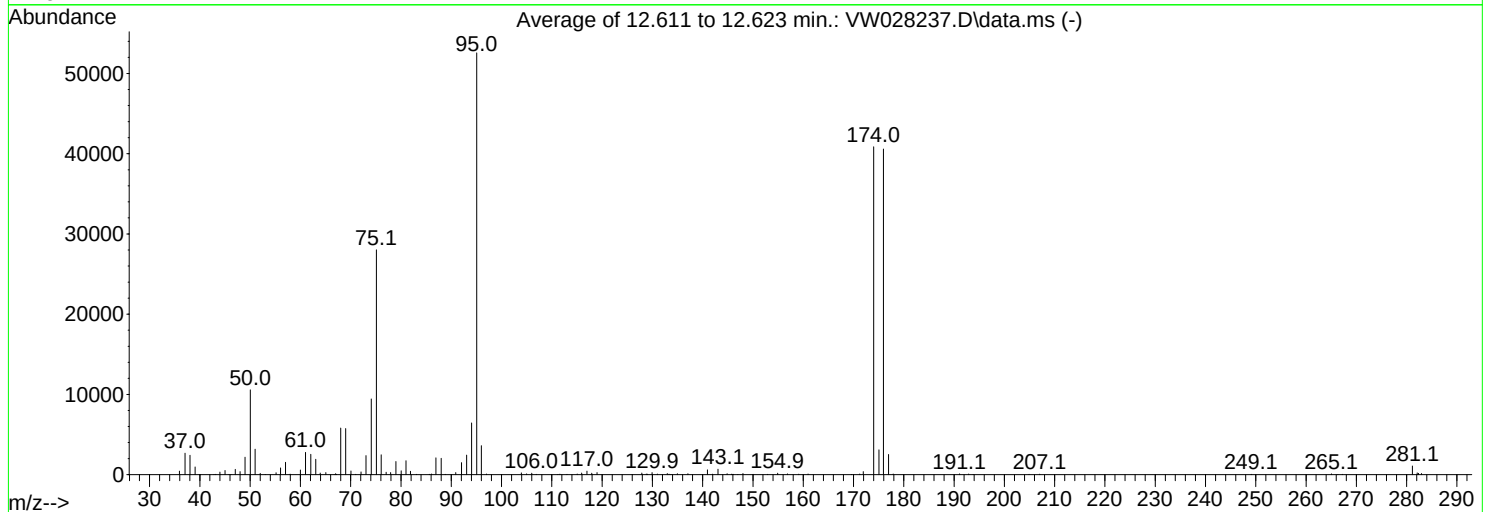


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032524\
Data File : VW028237.D
Acq On : 25 Mar 2024 08:31
Operator : SY/MD
Sample : BFB458
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB458

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Title : SFAM01.0
Last Update : Tue Mar 26 01:17:39 2024

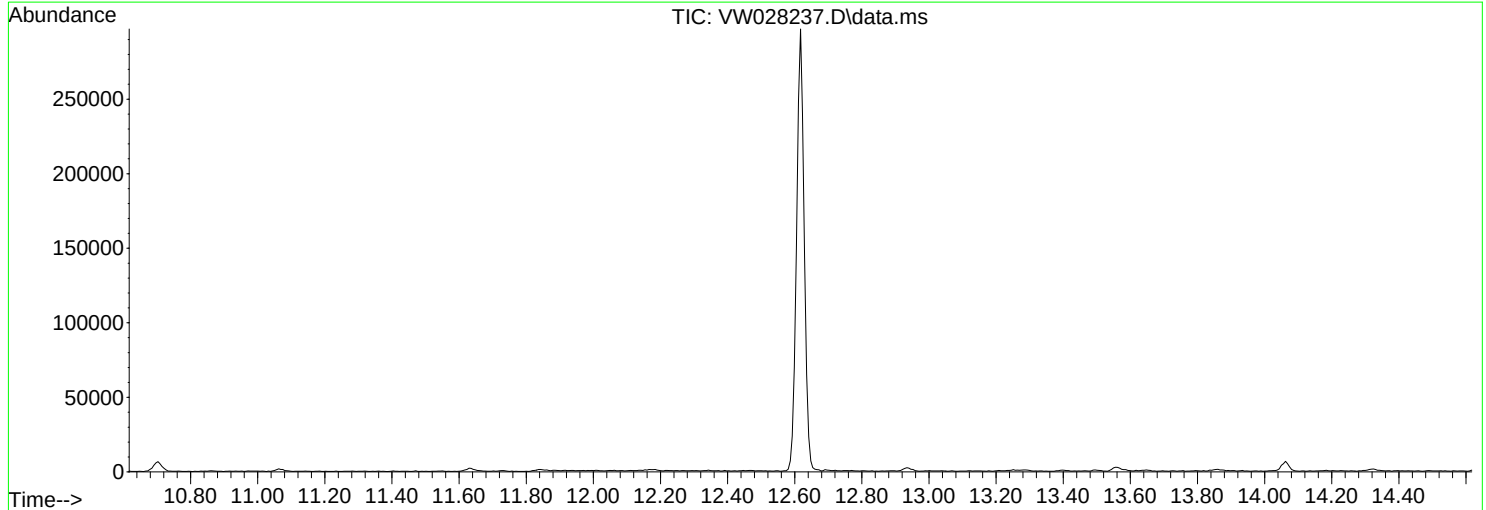

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	10567	PASS
75	95	30	80	53.3	28013	PASS
95	95	100	100	100.0	52571	PASS
96	95	5	9	6.9	3612	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.7	40867	PASS
175	174	5	9	7.6	3091	PASS
176	174	95	101	99.3	40581	PASS
177	176	5	9	6.2	2506	PASS

m/z	Abundance
36.10	167.0
39.90	207.0
44.10	110.0
54.80	60.0

Instrument :
MSVOA_W
ClientSampleId :
BFB458

m/z	Abundance
36.00	676.0
37.00	2684.0
38.10	2517.0
39.10	909.0
40.00	209.0
43.20	55.0
43.90	431.0
45.00	567.0
45.80	66.0
47.10	718.0
48.10	367.0
49.00	2260.0
50.10	10397.0
51.00	3345.0
52.00	186.0
53.00	72.0
55.20	289.0
56.00	851.0
57.10	1355.0
57.90	77.0
60.00	640.0
61.00	2863.0
62.10	2753.0
63.10	2027.0
64.00	202.0
65.00	273.0
67.00	168.0
68.00	5931.0
69.00	5739.0
70.00	458.0
72.00	392.0
73.00	2376.0
74.10	8818.0
75.10	26680.0
76.00	2322.0
77.10	203.0
77.90	197.0
79.00	1639.0
80.00	487.0
81.00	1706.0
81.90	397.0
85.60	51.0
86.10	86.0
87.00	2160.0
88.00	1962.0
88.80	114.0
90.80	208.0
92.00	1421.0
93.00	2151.0
94.00	6209.0
95.00	50512.0
96.00	3564.0
103.90	191.0
104.90	66.0
106.10	135.0
111.20	52.0
111.70	51.0
115.10	74.0
115.90	238.0
117.00	402.0
118.00	206.0
119.00	256.0
126.00	59.0
127.90	266.0
128.80	97.0
129.90	199.0
130.90	55.0
133.00	265.0
133.70	74.0
134.90	81.0
137.10	136.0
141.00	530.0
143.10	703.0
144.80	72.0
145.80	84.0
147.00	83.0
148.00	94.0
150.10	59.0
152.90	64.0
155.00	192.0
156.80	111.0
159.10	64.0
161.00	86.0
171.90	369.0
174.00	35480.0
175.00	2824.0
175.90	36048.0
177.00	2252.0
177.90	81.0
191.20	168.0
192.90	191.0
193.80	86.0

Instrument :
MSVOA_W
ClientSampleId :
BFB458

204.90	54.0
207.10	111.0
249.10	124.0
265.10	197.0
266.30	56.0
267.30	57.0
281.10	1766.0
282.10	530.0
282.90	251.0

Instrument :
MSVOA_W
ClientSampleId :
BFB458

m/z	Abundance
35.90	643.0
37.10	3013.0
38.00	2637.0
39.00	1217.0
39.90	233.0
43.10	78.0
44.00	571.0
45.00	522.0
47.10	640.0
48.00	395.0
49.00	2400.0
50.00	11772.0
51.00	3294.0
52.00	205.0
55.20	276.0
56.10	940.0
57.00	1716.0
60.00	547.0
61.00	3194.0
62.00	2722.0
63.10	2071.0
63.90	198.0
65.10	258.0
67.00	193.0
68.00	6383.0
69.00	6371.0
70.00	584.0
71.00	58.0
72.10	364.0
73.10	2580.0
74.10	10462.0
75.10	32016.0
76.00	2895.0
77.00	358.0
77.90	275.0
79.00	1888.0
80.10	542.0
81.00	2041.0
81.90	436.0
83.10	53.0
85.70	93.0
86.90	2229.0
88.00	2351.0
90.90	303.0
92.10	1746.0
93.10	2818.0
94.10	7198.0
95.00	59360.0
96.00	4085.0
97.00	120.0
103.90	243.0
105.00	129.0
106.00	258.0
106.90	54.0
111.60	67.0
113.00	76.0
114.90	81.0
115.90	230.0
117.00	468.0
117.90	130.0
119.10	312.0
127.90	224.0
128.80	134.0
130.00	222.0
131.00	95.0
132.90	145.0
133.30	173.0
134.90	165.0
137.10	128.0
140.90	647.0
142.00	117.0
143.00	785.0
144.90	187.0
145.70	80.0
146.10	97.0
148.00	158.0
149.90	55.0
152.90	66.0
154.80	180.0
156.90	107.0
159.10	97.0
161.00	79.0
171.30	152.0
172.00	391.0
174.00	47208.0
175.10	3452.0
176.00	47616.0
176.90	2873.0
177.90	71.0
191.00	156.0
192.90	66.0
204.90	53.0

Instrument :
MSVOA_W
ClientSampleId :
BFB458

207.00	62.0
264.90	108.0
267.10	62.0
281.20	961.0
282.30	359.0
283.00	147.0

Instrument :
MSVOA_W
ClientSampleId :
BFB458

m/z	Abundance
36.00	485.0
37.10	2315.0
38.00	2089.0
39.00	747.0
40.00	211.0
42.80	81.0
44.10	312.0
45.00	454.0
46.20	66.0
47.00	616.0
47.90	383.0
49.00	1894.0
50.00	9533.0
51.00	2896.0
52.00	110.0
55.00	171.0
56.10	703.0
57.00	1539.0
58.00	108.0
60.00	531.0
61.00	2287.0
62.00	2151.0
63.00	1669.0
64.00	219.0
65.00	243.0
66.70	81.0
67.20	98.0
68.00	5097.0
69.00	5130.0
70.10	364.0
71.00	53.0
72.10	258.0
73.00	2191.0
74.10	9036.0
75.10	25344.0
76.10	2229.0
77.00	364.0
78.00	304.0
79.00	1400.0
80.00	398.0
81.00	1450.0
81.90	413.0
83.10	54.0
86.10	150.0
87.00	1908.0
88.00	1815.0
91.00	289.0
92.00	1297.0
93.00	2315.0
94.10	5916.0
95.10	47840.0
96.00	3188.0
97.00	144.0
104.00	254.0
105.10	85.0
105.90	167.0
106.90	60.0
111.50	71.0
113.00	75.0
115.10	72.0
116.00	163.0
117.00	477.0
118.00	189.0
118.90	231.0
127.80	144.0
129.00	162.0
129.80	170.0
130.10	170.0
131.10	77.0
135.00	90.0
136.90	102.0
141.00	610.0
141.90	81.0
143.00	544.0
144.90	91.0
145.90	95.0
148.00	163.0
154.90	180.0
156.90	96.0
160.90	69.0
169.60	59.0
171.20	93.0
172.00	390.0
174.00	39912.0
175.00	2996.0
176.00	38080.0
177.00	2394.0
177.90	107.0
281.20	514.0
282.00	117.0
282.40	150.0

Instrument :
MSVOA_W
ClientSampleId :
BFB458