

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032724\
 Data File : VW028246.D
 Acq On : 27 Mar 2024 10:50
 Operator : SY/MD
 Sample : P1839-12
 Misc : 5.10g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Mar 28 01:12:17 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 28 01:11:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	194811	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	184920	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	90471	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	44246	19.411	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	77.640%		
7) Chloroethane-d5	2.899	69	35165	22.082	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	88.320%		
11) 1,1-Dichloroethene-d2	4.027	65	30009	20.761	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	83.040%		
21) 2-Butanone-d5	7.081	46	34419	51.197	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	102.400%		
24) Chloroform-d	7.648	84	142575	24.819	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	99.280%		
26) 1,2-Dichloroethane-d4	8.307	65	80243	25.348	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	101.400%		
32) Benzene-d6	8.276	84	276356	24.478	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	97.920%		
36) 1,2-Dichloropropane-d6	9.276	67	81690	25.143	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	100.560%		
41) Toluene-d8	10.319	98	251116	24.114	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	96.440%		
43) trans-1,3-Dichloroprop...	10.575	79	34058	23.080	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	92.320%		
47) 2-Hexanone-d5	10.922	63	26222	48.826	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	97.660%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	59909	24.962	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	99.840%		
66) 1,2-Dichlorobenzene-d4	13.848	152	86656	26.294	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	105.160%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.038	75	2602	0.558	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032724\
Data File : VW028246.D
Acq On : 27 Mar 2024 10:50
Operator : SY/MD
Sample : P1839-12
Misc : 5.10g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Mar 28 01:12:17 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 28 01:11:29 2024
Response via : Initial Calibration

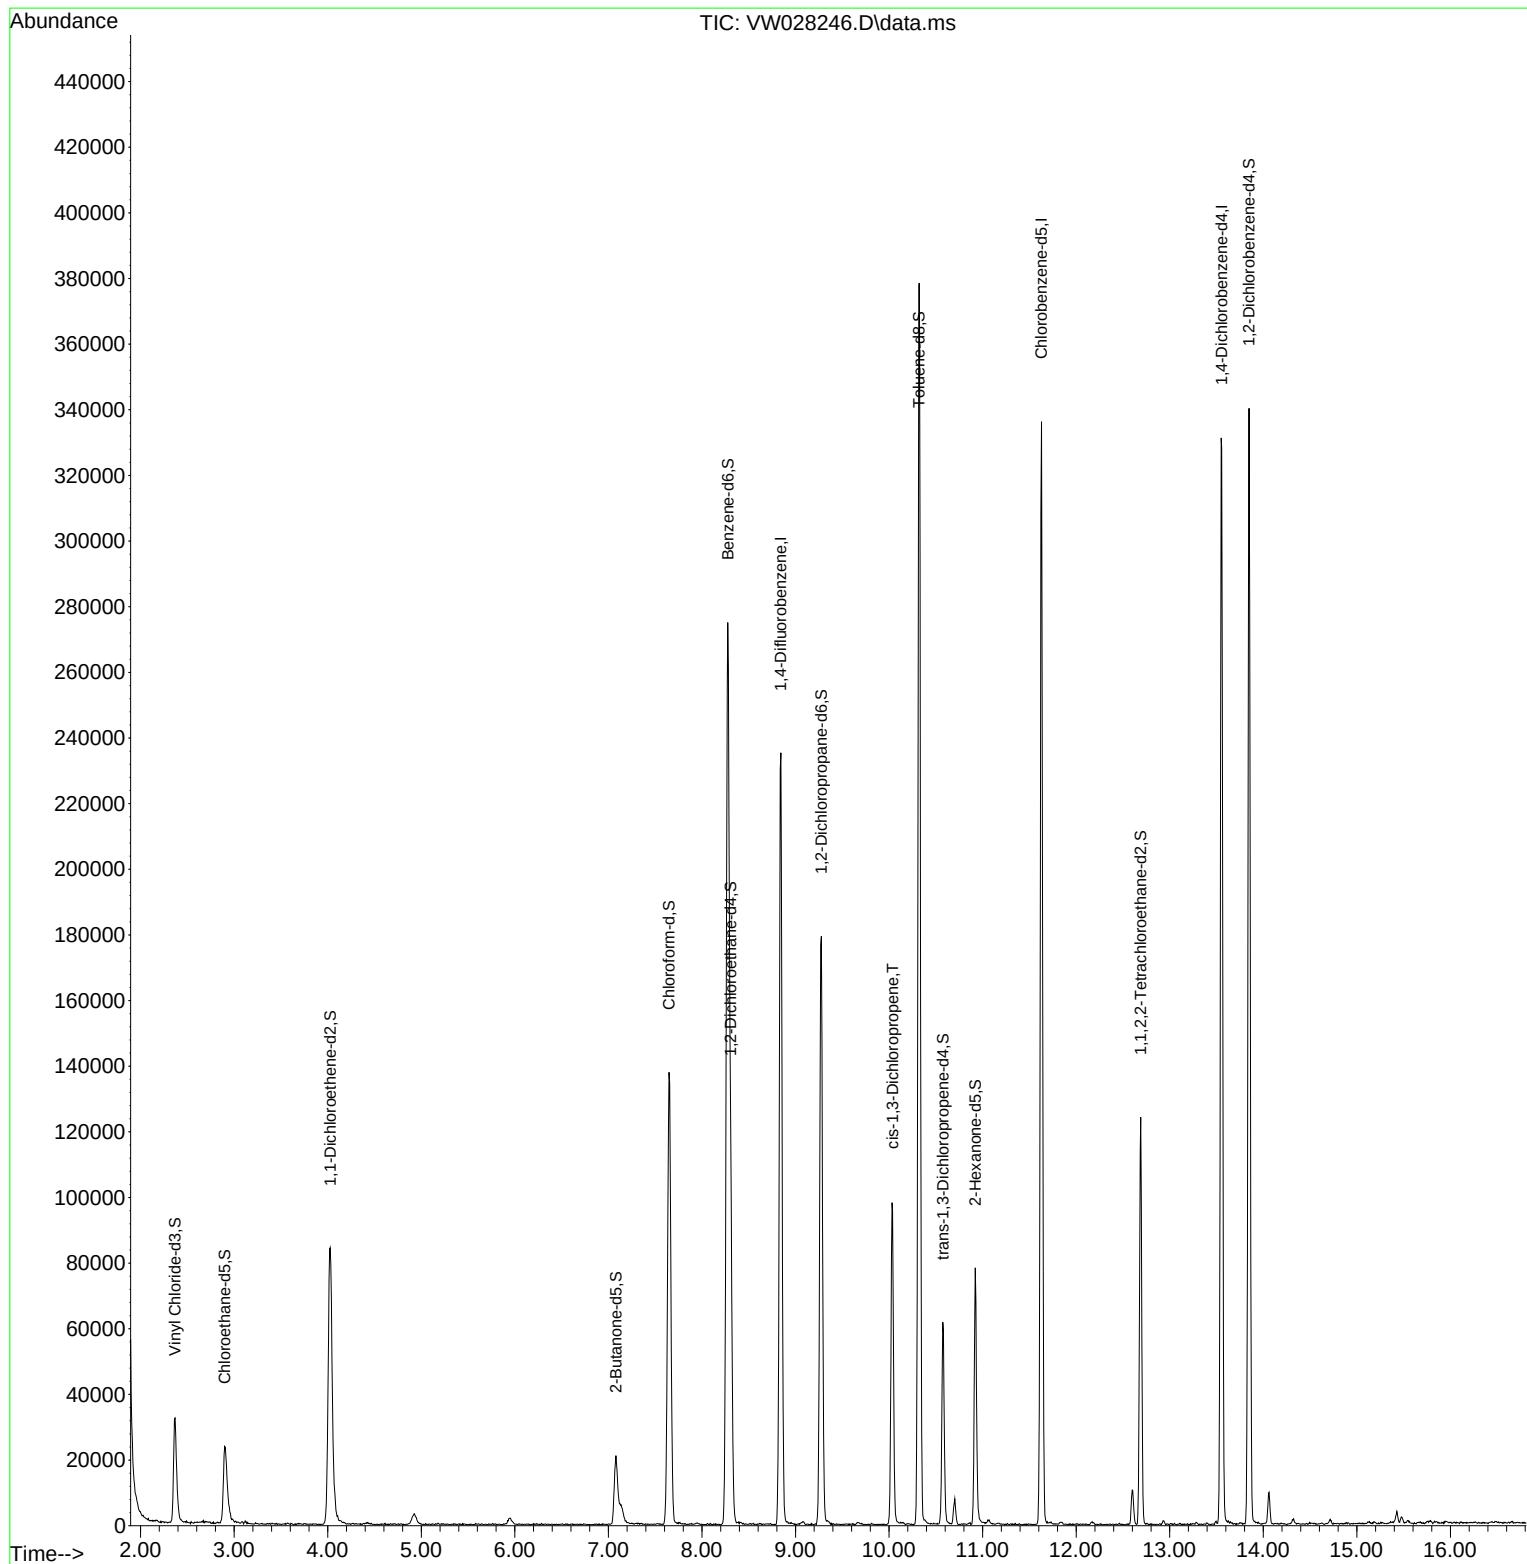

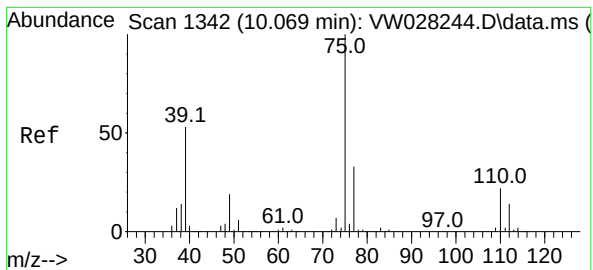

#39
 cis-1,3-Dichloropropene
 Concen: 0.558 ug/L
 RT: 10.038 min Scan# 14
 Delta R.T. -0.031 min
 Lab File: VW028246.D
 Acq: 27 Mar 2024 10:50

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion:	75	Resp:	2602
Ion Ratio	Lower	Upper	
75	100		
77	39.0	22.5	41.7

