


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032724\
Data File : VW028243.D
Acq On : 27 Mar 2024 08:54
Operator : SY/MD
Sample : BFB459
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB459

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Title : SFAM01.0
Last Update : Thu Mar 28 01:11:29 2024

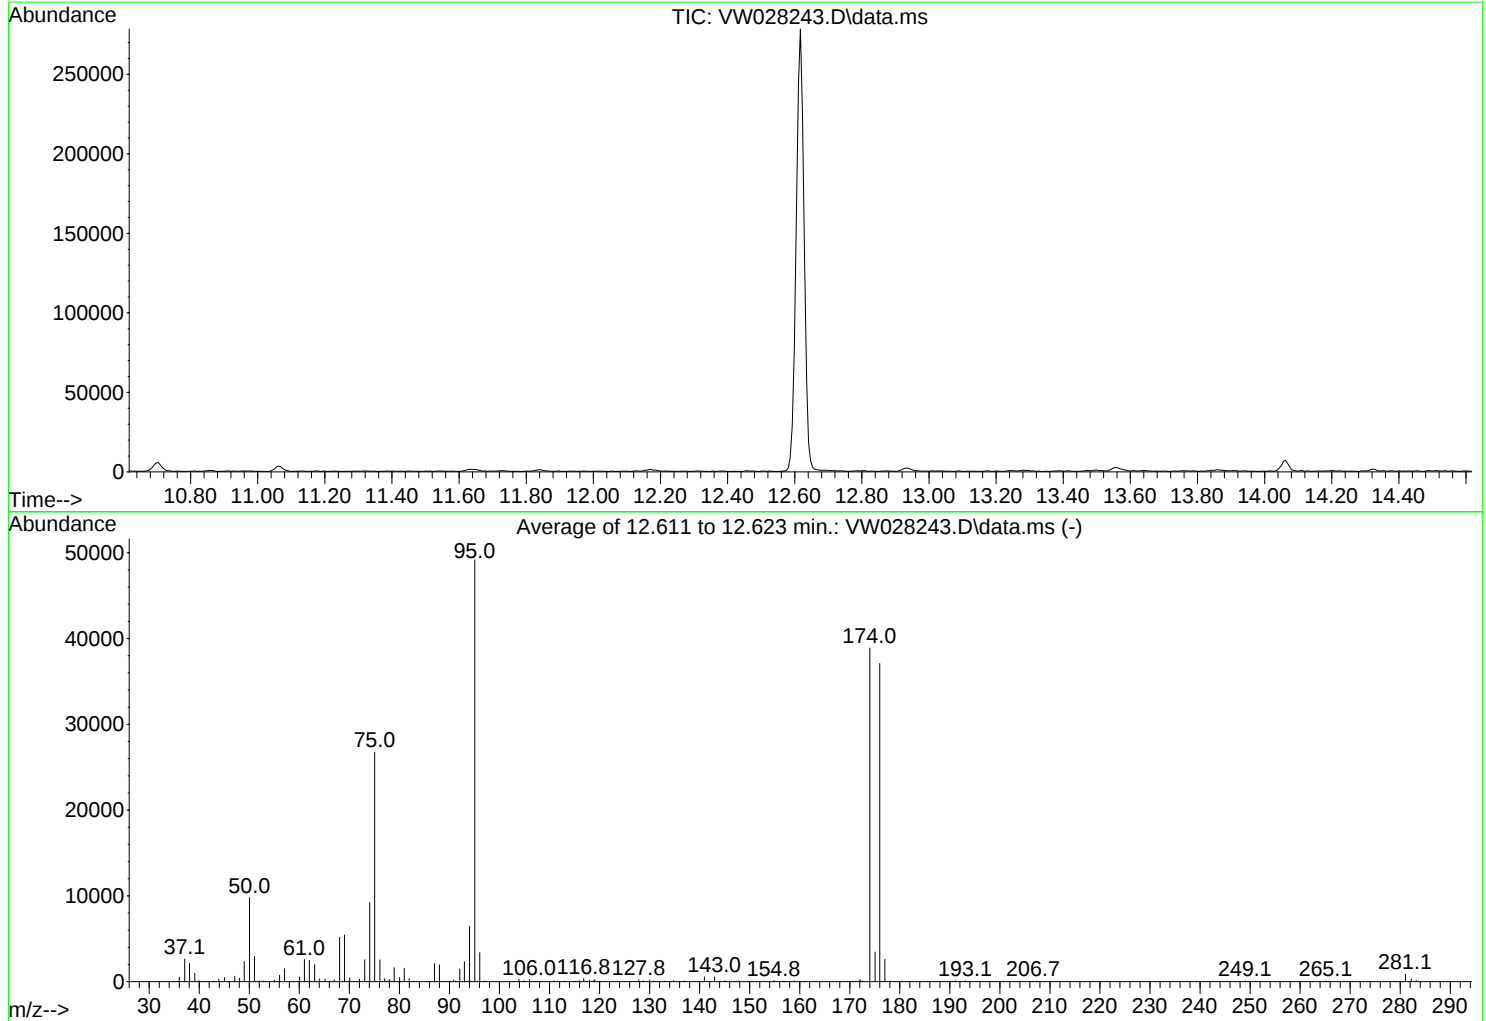

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	9788	PASS
75	95	30	80	54.4	26744	PASS
95	95	100	100	100.0	49179	PASS
96	95	5	9	6.9	3369	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.1	38893	PASS
175	174	5	9	8.9	3454	PASS
176	174	95	101	95.4	37088	PASS
177	176	5	9	7.0	2605	PASS

m/z	Abundance
38.30	56.0
40.00	182.0
43.90	130.0

Instrument :
MSVOA_W
ClientSampleId :
BFB459

m/z	Abundance
36.00	557.0
37.10	2903.0
38.10	2006.0
39.10	1143.0
39.90	308.0
43.20	71.0
43.90	384.0
45.00	562.0
45.90	66.0
47.10	698.0
48.10	472.0
49.00	2431.0
50.00	10054.0
51.00	3043.0
52.00	129.0
52.90	61.0
55.10	213.0
56.00	682.0
57.10	1344.0
58.00	70.0
60.10	541.0
61.00	2634.0
62.00	2394.0
63.10	2042.0
64.20	306.0
65.10	283.0
66.90	184.0
68.10	5192.0
69.00	5473.0
70.00	445.0
72.00	328.0
73.00	2659.0
74.10	9552.0
75.10	26760.0
76.10	2569.0
77.10	309.0
78.10	231.0
78.90	1694.0
80.10	612.0
81.00	1533.0
82.00	290.0
87.00	1923.0
88.00	2061.0
90.90	209.0
92.00	1468.0
93.00	2068.0
94.00	6302.0
95.00	49120.0
96.00	3297.0
103.00	59.0
104.00	278.0
104.80	109.0
106.00	269.0
106.80	80.0
109.90	81.0
110.90	86.0
113.10	79.0
114.90	141.0
116.00	190.0
116.90	386.0
118.00	174.0
118.80	349.0
123.80	75.0
127.90	175.0
128.90	67.0
130.00	173.0
131.10	58.0
133.10	113.0
134.10	103.0
134.90	161.0
136.90	91.0
139.90	104.0
141.00	698.0
143.00	594.0
144.10	74.0
145.00	194.0
146.00	83.0
147.90	108.0
149.80	62.0
155.00	94.0
156.80	117.0
158.90	80.0
171.20	84.0
171.90	416.0
172.50	309.0
174.00	34848.0
175.10	3302.0
176.00	34184.0
177.00	2452.0
178.10	89.0
191.20	155.0
192.10	67.0

Instrument :
MSVOA_W
ClientSampleId :
BFB459

193.10	243.0
206.70	119.0
249.10	126.0
251.20	69.0
265.20	140.0
281.10	1403.0
282.20	483.0
283.20	236.0
284.30	87.0

Instrument :
MSVOA_W
ClientSampleId :
BFB459

m/z	Abundance
36.00	571.0
37.10	2827.0
38.00	2300.0
39.10	1031.0
40.00	336.0
44.00	416.0
45.10	500.0
46.20	63.0
47.10	680.0
48.00	412.0
49.00	2727.0
50.10	10808.0
51.10	3353.0
52.00	214.0
52.90	54.0
55.00	232.0
56.10	916.0
57.10	1852.0
58.20	87.0
60.00	578.0
61.00	2850.0
62.00	2801.0
63.00	2287.0
64.00	344.0
65.20	331.0
66.20	102.0
67.00	208.0
68.00	6065.0
69.00	6457.0
70.10	465.0
72.00	284.0
73.10	2830.0
74.10	10199.0
75.10	29752.0
76.10	2939.0
77.00	402.0
77.70	273.0
78.10	266.0
79.00	1752.0
80.10	454.0
80.90	1715.0
81.90	373.0
85.80	77.0
87.00	2599.0
88.00	2097.0
90.80	208.0
91.20	180.0
92.10	1817.0
93.00	2896.0
94.00	7380.0
95.10	53848.0
96.10	3901.0
97.00	112.0
97.30	88.0
103.90	315.0
104.90	139.0
105.90	318.0
107.20	78.0
110.90	132.0
112.90	96.0
115.10	98.0
116.10	171.0
116.80	390.0
118.00	236.0
119.00	447.0
125.00	57.0
127.80	278.0
128.80	93.0
129.90	248.0
130.80	106.0
132.90	85.0
134.80	121.0
137.00	103.0
139.90	57.0
141.00	535.0
141.90	95.0
143.00	682.0
144.00	51.0
145.20	119.0
146.00	67.0
147.80	94.0
149.90	54.0
153.90	50.0
154.80	130.0
157.00	106.0
158.90	121.0
161.20	101.0
170.50	80.0
172.10	334.0
174.00	43416.0
175.10	3931.0
176.00	41440.0

Instrument :
MSVOA_W
ClientSampleId :
BFB459

177.00	2933.0
178.10	96.0
191.10	126.0
192.80	135.0
206.70	52.0
207.30	101.0
249.00	112.0
265.10	170.0
281.00	868.0
282.20	389.0
283.20	188.0
284.00	53.0

Instrument :
MSVOA_W
ClientSampleId :
BFB459

m/z	Abundance
36.00	457.0
37.10	2205.0
38.00	2089.0
39.00	718.0
40.00	289.0
41.10	63.0
42.80	59.0
44.00	405.0
45.00	359.0
46.00	71.0
47.10	503.0
48.00	360.0
49.00	1819.0
50.00	8503.0
51.10	2534.0
52.20	112.0
52.90	95.0
54.90	94.0
56.10	671.0
57.00	1349.0
58.00	76.0
60.00	482.0
61.00	2218.0
62.00	2278.0
63.00	1683.0
63.90	158.0
64.10	159.0
65.10	283.0
66.10	64.0
67.00	214.0
68.00	4272.0
69.10	4430.0
70.00	369.0
72.00	308.0
73.10	2170.0
74.00	7928.0
75.00	23720.0
76.10	2102.0
77.00	290.0
78.00	267.0
79.00	1444.0
79.90	411.0
80.90	1460.0
81.90	383.0
82.90	64.0
86.10	102.0
87.00	1731.0
88.00	1663.0
90.80	217.0
92.00	1125.0
93.00	2012.0
94.00	5657.0
95.00	44568.0
96.10	2910.0
97.00	60.0
97.30	63.0
103.80	234.0
105.00	82.0
106.10	152.0
110.90	57.0
115.10	86.0
115.80	131.0
116.90	305.0
118.00	162.0
119.10	266.0
127.90	236.0
128.70	120.0
129.70	124.0
130.10	151.0
130.80	51.0
134.70	89.0
135.10	80.0
136.90	109.0
140.80	445.0
142.00	98.0
143.00	431.0
144.90	133.0
145.80	88.0
147.20	53.0
147.80	115.0
149.80	69.0
154.80	153.0
158.90	59.0
161.10	62.0
170.70	96.0
172.00	334.0
174.00	38416.0
175.00	3129.0
176.00	35640.0
177.00	2430.0
177.90	104.0
193.20	55.0

Instrument :
MSVOA_W
ClientSampleId :
BFB459

264.80	63.0
281.00	289.0
282.20	81.0
283.10	53.0

Instrument :
MSVOA_W
ClientSampleId :
BFB459