

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032824\
 Data File : VW028268.D
 Acq On : 28 Mar 2024 14:17
 Operator : SY/MD
 Sample : P1886-18
 Misc : 4.84g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Mar 28 23:33:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 28 23:31:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	433084	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	395714	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	183542	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	71171	14.045	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.200%
7) Chloroethane-d5	2.899	69	55831	15.770	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	63.080%
11) 1,1-Dichloroethene-d2	4.027	65	45926	14.292	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.160%
21) 2-Butanone-d5	7.075	46	65286	43.683	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.360%
24) Chloroform-d	7.648	84	209386	16.396	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	65.600%
26) 1,2-Dichloroethane-d4	8.307	65	116287	16.524	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	66.080%#
32) Benzene-d6	8.276	84	419228	17.352	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	69.400%
36) 1,2-Dichloropropane-d6	9.270	67	127516	18.341	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	73.360%
41) Toluene-d8	10.325	98	373471	16.759	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	67.040%
43) trans-1,3-Dichloroprop...	10.575	79	52925	16.760	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	67.040%
47) 2-Hexanone-d5	10.922	63	53612	46.650	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.300%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	99661	19.405	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	77.600%
66) 1,2-Dichlorobenzene-d4	13.848	152	120112	17.964	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	71.840%#
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	3659	0.367	ug/L	Qvalue # 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032824\
Data File : VW028268.D
Acq On : 28 Mar 2024 14:17
Operator : SY/MD
Sample : P1886-18
Misc : 4.84g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Mar 28 23:33:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 28 23:31:04 2024
Response via : Initial Calibration

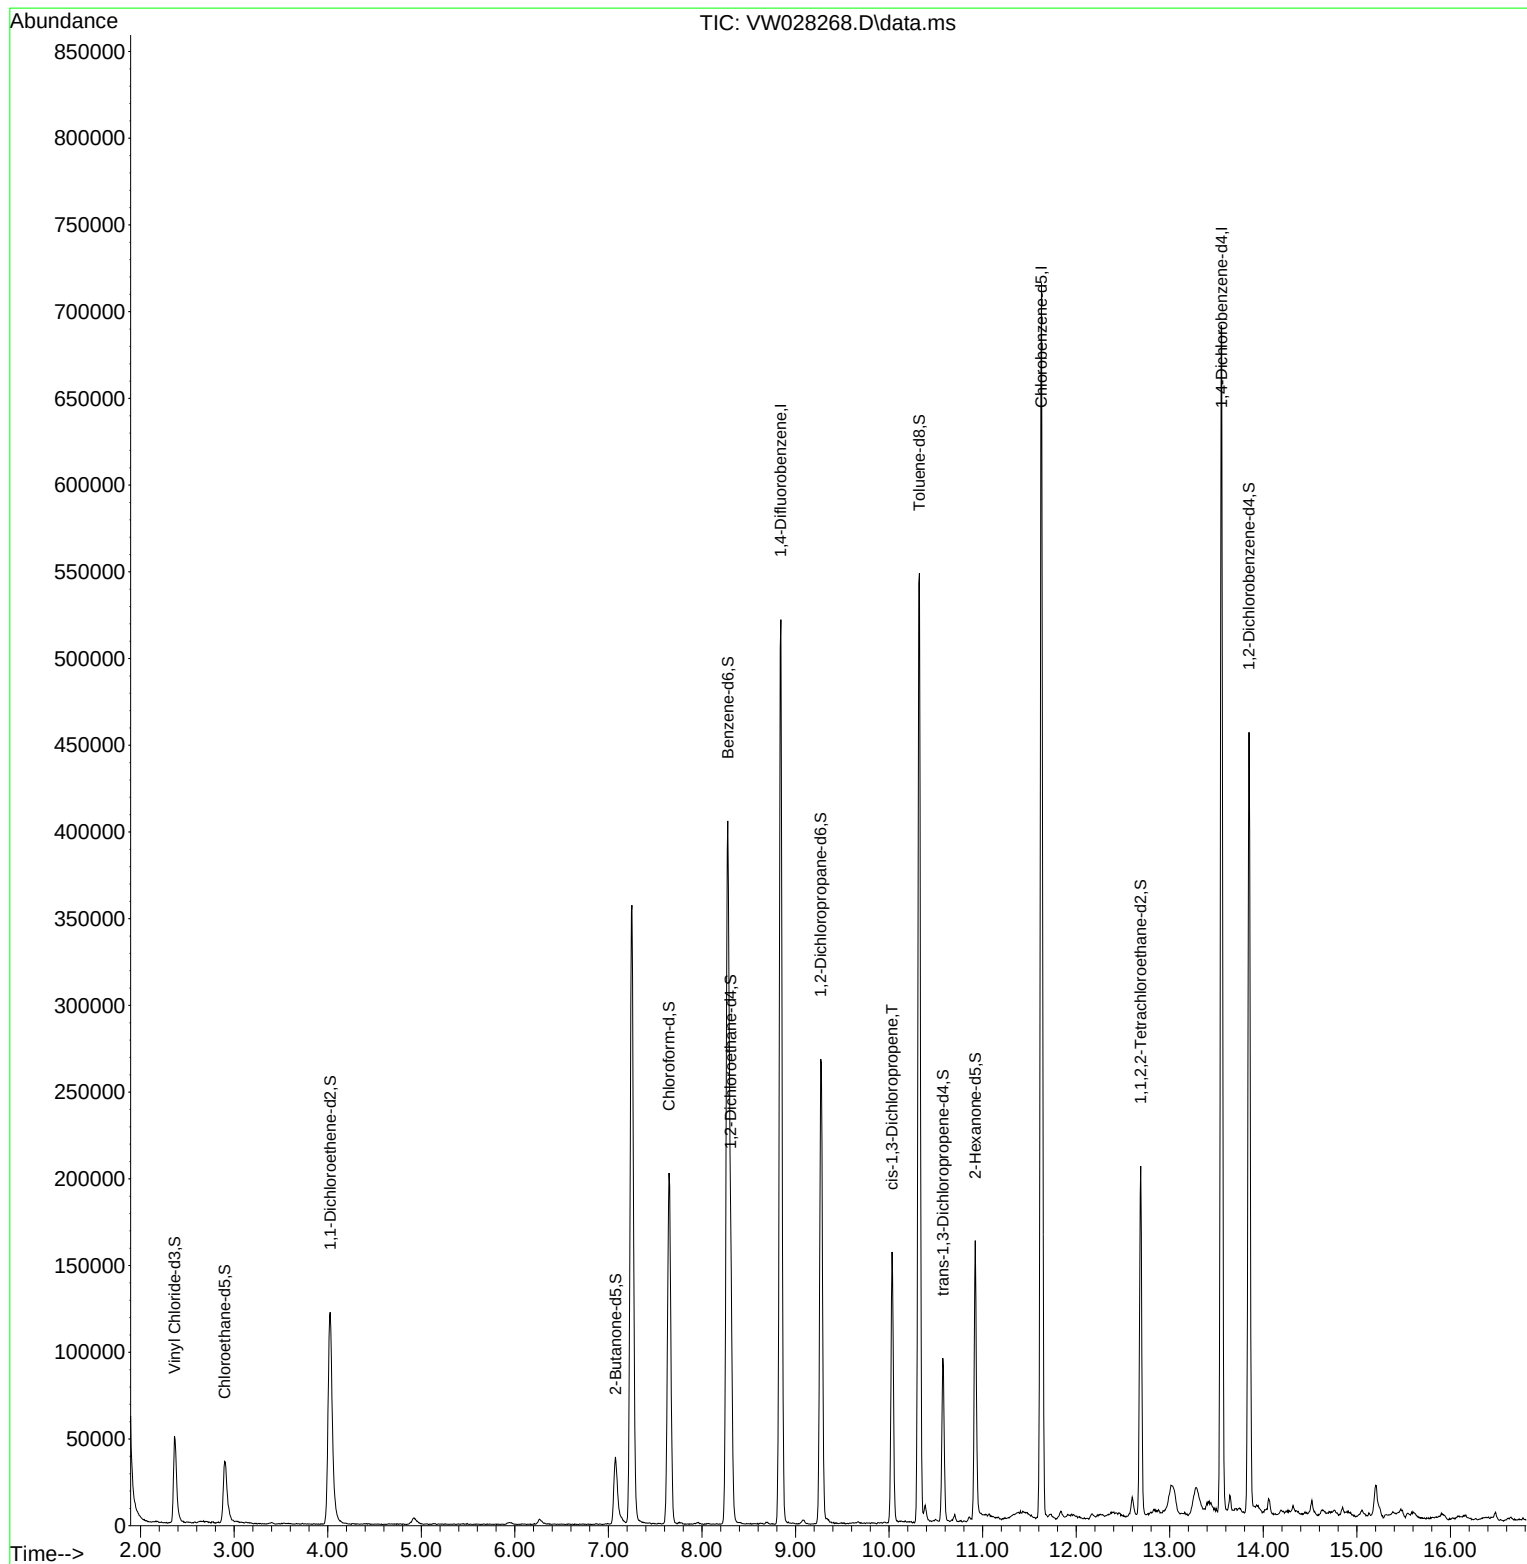

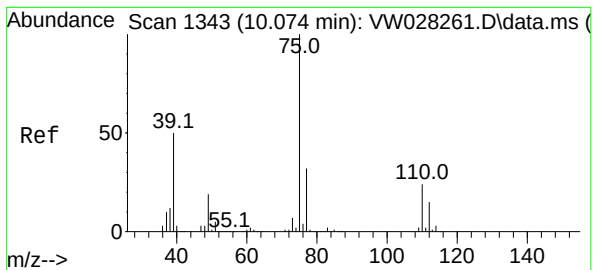

#39
cis-1,3-Dichloropropene
Concen: 0.367 ug/L
RT: 10.032 min Scan# 14
Delta R.T. -0.042 min
Lab File: VW028268.D
Acq: 28 Mar 2024 14:17

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 75 Resp: 3659
Ion Ratio Lower Upper
75 100
77 50.7 22.5 41.7#

