
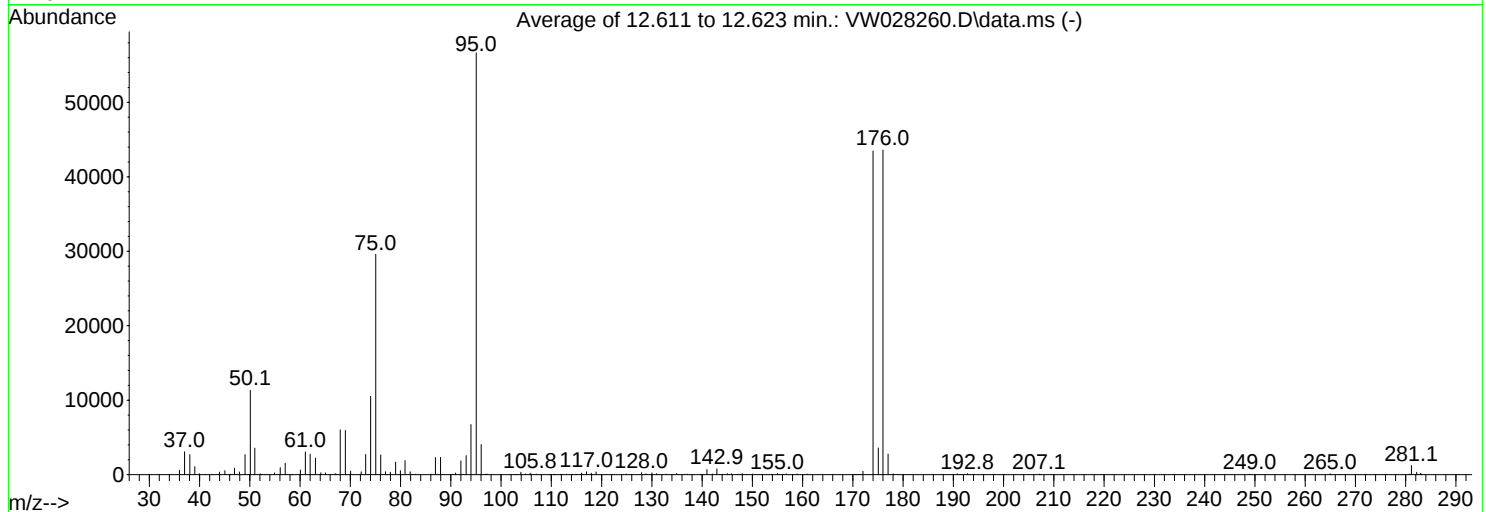


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032824\
Data File : VW028260.D
Acq On : 28 Mar 2024 08:23
Operator : SY/MD
Sample : BFB460
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB460

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Title : SFAM01.0
Last Update : Thu Mar 28 23:31:04 2024

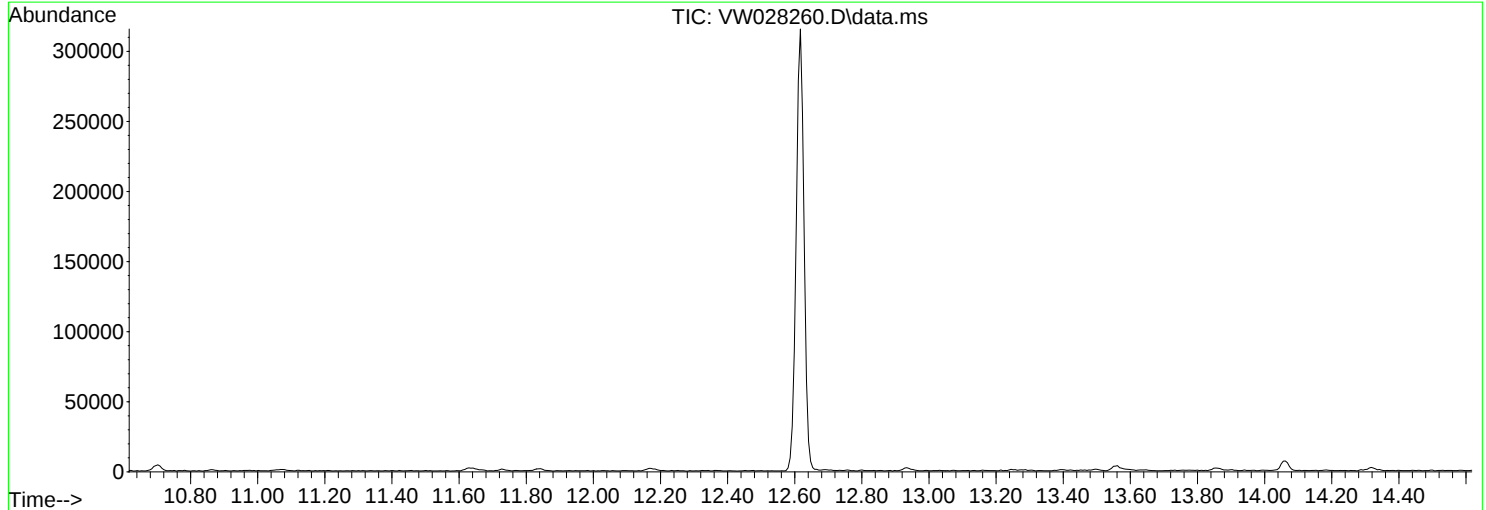

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	11334	PASS
75	95	30	80	52.2	29584	PASS
95	95	100	100	100.0	56651	PASS
96	95	5	9	7.1	4049	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.7	43475	PASS
175	174	5	9	8.2	3586	PASS
176	174	95	101	100.3	43603	PASS
177	176	5	9	6.4	2770	PASS

m/z	Abundance
37.70	54.0
39.90	443.0
43.90	104.0
44.30	71.0

Instrument :
MSVOA_W
ClientSampleId :
BFB460

m/z	Abundance
36.00	637.0
37.00	3381.0
38.00	3068.0
39.10	1154.0
40.00	654.0
44.10	434.0
45.00	618.0
47.00	882.0
48.00	411.0
49.00	2611.0
50.10	11513.0
51.00	3489.0
52.20	152.0
53.10	74.0
54.90	240.0
56.00	1093.0
57.00	1416.0
60.10	654.0
61.00	3162.0
62.00	2908.0
63.00	2353.0
64.20	302.0
65.00	270.0
67.00	230.0
68.00	6239.0
69.00	6194.0
70.00	444.0
72.10	378.0
73.10	2899.0
74.10	10297.0
75.10	29928.0
76.10	2778.0
77.10	354.0
78.00	351.0
79.00	1748.0
80.10	518.0
80.90	1904.0
81.90	403.0
87.00	2425.0
87.90	2425.0
91.10	195.0
92.00	1568.0
93.10	2512.0
94.00	6891.0
95.10	55056.0
96.00	4310.0
96.90	200.0
102.90	84.0
104.00	332.0
104.90	102.0
105.80	261.0
106.90	111.0
109.70	60.0
110.70	74.0
111.90	68.0
115.00	83.0
116.00	331.0
117.00	347.0
117.90	193.0
119.00	354.0
125.00	152.0
127.90	198.0
128.90	88.0
130.00	187.0
131.00	181.0
132.90	199.0
135.10	96.0
137.10	84.0
139.70	53.0
140.90	634.0
142.10	69.0
143.00	850.0
145.00	135.0
145.80	129.0
147.00	62.0
148.10	92.0
148.80	74.0
150.00	60.0
154.00	74.0
155.00	100.0
156.80	122.0
158.90	64.0
161.00	107.0
162.90	57.0
170.50	61.0
171.90	443.0
174.00	40696.0
175.00	3516.0
176.00	39152.0
177.00	2878.0
178.00	106.0
179.10	55.0

Instrument :
MSVOA_W
ClientSampleId :
BFB460

190.80	134.0
191.40	114.0
192.90	202.0
194.00	64.0
207.10	134.0
249.00	102.0
265.10	192.0
266.80	55.0
281.20	2058.0
282.30	510.0
283.00	302.0

Instrument :
MSVOA_W
ClientSampleId :
BFB460

m/z	Abundance
36.00	712.0
37.00	3384.0
38.00	2823.0
39.10	1198.0
40.00	598.0
41.20	55.0
42.70	55.0
44.00	526.0
45.10	581.0
46.20	85.0
47.00	836.0
48.00	323.0
49.10	3093.0
50.10	12609.0
51.00	4035.0
52.00	158.0
53.00	75.0
55.00	266.0
56.10	942.0
57.10	1846.0
60.00	667.0
61.10	3399.0
62.00	2817.0
63.00	2398.0
64.00	231.0
65.10	222.0
67.20	200.0
68.00	6469.0
69.00	6286.0
70.10	601.0
72.10	437.0
73.00	2791.0
74.00	12302.0
75.00	33248.0
76.10	2904.0
77.00	445.0
77.90	292.0
79.00	1768.0
79.90	528.0
80.90	2103.0
81.90	411.0
83.00	86.0
87.00	2426.0
88.00	2419.0
90.90	261.0
92.00	2141.0
93.00	2980.0
94.00	7530.0
95.00	64888.0
96.00	4487.0
97.20	152.0
103.20	58.0
103.90	313.0
104.80	81.0
105.80	293.0
107.00	83.0
110.70	73.0
111.80	86.0
113.10	113.0
114.80	113.0
116.10	178.0
117.00	400.0
117.90	183.0
118.90	469.0
124.90	108.0
126.00	85.0
128.00	301.0
128.90	173.0
130.00	357.0
130.90	153.0
134.90	173.0
136.60	104.0
137.20	85.0
141.00	817.0
141.90	106.0
143.00	725.0
144.00	79.0
145.10	109.0
145.90	117.0
147.00	70.0
147.90	194.0
150.10	64.0
153.80	67.0
155.00	181.0
156.10	63.0
156.70	92.0
159.00	125.0
160.80	112.0
170.80	103.0
172.00	501.0
174.00	47744.0
175.10	3797.0

Instrument :
MSVOA_W
ClientSampleId :
BFB460

176.00	49200.0
177.00	2982.0
178.10	121.0
190.80	112.0
192.70	131.0
193.30	137.0
207.30	87.0
249.00	111.0
264.90	141.0
281.10	1097.0
282.10	331.0
282.90	152.0
283.20	164.0

Instrument :
MSVOA_W
ClientSampleId :
BFB460

m/z	Abundance
36.10	443.0
37.00	2429.0
38.10	2174.0
39.00	854.0
40.00	467.0
43.90	371.0
45.10	384.0
46.10	90.0
46.90	856.0
47.90	341.0
49.00	2376.0
50.10	9879.0
51.00	3208.0
52.30	132.0
54.90	211.0
56.10	791.0
57.00	1342.0
58.30	76.0
60.10	544.0
61.00	2597.0
62.00	2548.0
63.10	1873.0
64.20	249.0
65.00	217.0
67.00	146.0
68.00	5354.0
69.00	5291.0
70.10	354.0
72.20	329.0
73.00	2419.0
74.10	8920.0
75.10	25576.0
76.00	2235.0
76.90	340.0
77.90	354.0
79.00	1534.0
79.90	547.0
80.90	1694.0
81.90	358.0
82.90	90.0
86.10	193.0
86.90	2061.0
87.90	2154.0
90.90	222.0
92.00	1818.0
93.10	2158.0
94.00	5781.0
95.00	50008.0
96.10	3350.0
97.20	132.0
104.00	309.0
105.00	116.0
106.00	222.0
107.10	60.0
110.00	58.0
110.70	60.0
113.00	64.0
115.10	86.0
116.00	149.0
117.00	436.0
118.00	175.0
118.80	306.0
126.00	56.0
127.90	271.0
128.80	139.0
130.00	166.0
130.90	89.0
135.00	168.0
137.00	51.0
139.70	91.0
141.00	610.0
142.10	91.0
142.90	739.0
144.10	64.0
145.00	127.0
145.90	67.0
147.60	88.0
148.10	136.0
150.00	116.0
152.80	59.0
155.00	149.0
156.80	109.0
158.80	65.0
160.80	56.0
171.20	130.0
171.60	154.0
172.10	400.0
174.00	41984.0
175.00	3446.0
176.00	42456.0
177.00	2450.0
178.00	71.0

Instrument :
MSVOA_W
ClientSampleId :
BFB460

190.80	53.0
192.90	50.0
207.10	73.0
265.20	63.0
280.70	268.0
281.20	521.0
282.10	123.0
282.60	94.0
283.10	89.0

Instrument :
MSVOA_W
ClientSampleId :
BFB460