

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032923\
 Data File : VW025487.D
 Acq On : 29 Mar 2023 15:19
 Operator : SY/MD
 Sample : 02121-06
 Misc : 6.38g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Mar 30 00:23:23 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 30 00:21:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	955703	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	860629	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	404391	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	174950	11.010	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	44.040%
7) Chloroethane-d5	2.899	69	179975	15.741	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.960%
11) 1,1-Dichloroethene-d2	4.021	63	392686	12.795	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	51.160%
21) 2-Butanone-d5	7.075	46	192231	49.284	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.560%
24) Chloroform-d	7.648	84	608479	22.085	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.360%
26) 1,2-Dichloroethane-d4	8.057	65	221	0.015	ug/L	-0.25
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.276	84	1249495	21.248	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.000%
36) 1,2-Dichloropropane-d6	9.276	67	405752	22.303	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.200%
41) Toluene-d8	10.325	98	1107719	21.365	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.440%
43) trans-1,3-Dichloroprop...	10.575	79	157790	21.782	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.120%
47) 2-Hexanone-d5	10.922	63	124760	47.691	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.380%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	308327	23.134	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.520%
66) 1,2-Dichlorobenzene-d4	13.848	152	361163	24.016	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.080%
Target Compounds					Qvalue	
13) Acetone	4.124	43	24704	6.589	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032923\
Data File : VW025487.D
Acq On : 29 Mar 2023 15:19
Operator : SY/MD
Sample : 02121-06
Misc : 6.38g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Mar 30 00:23:23 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 30 00:21:45 2023
Response via : Initial Calibration

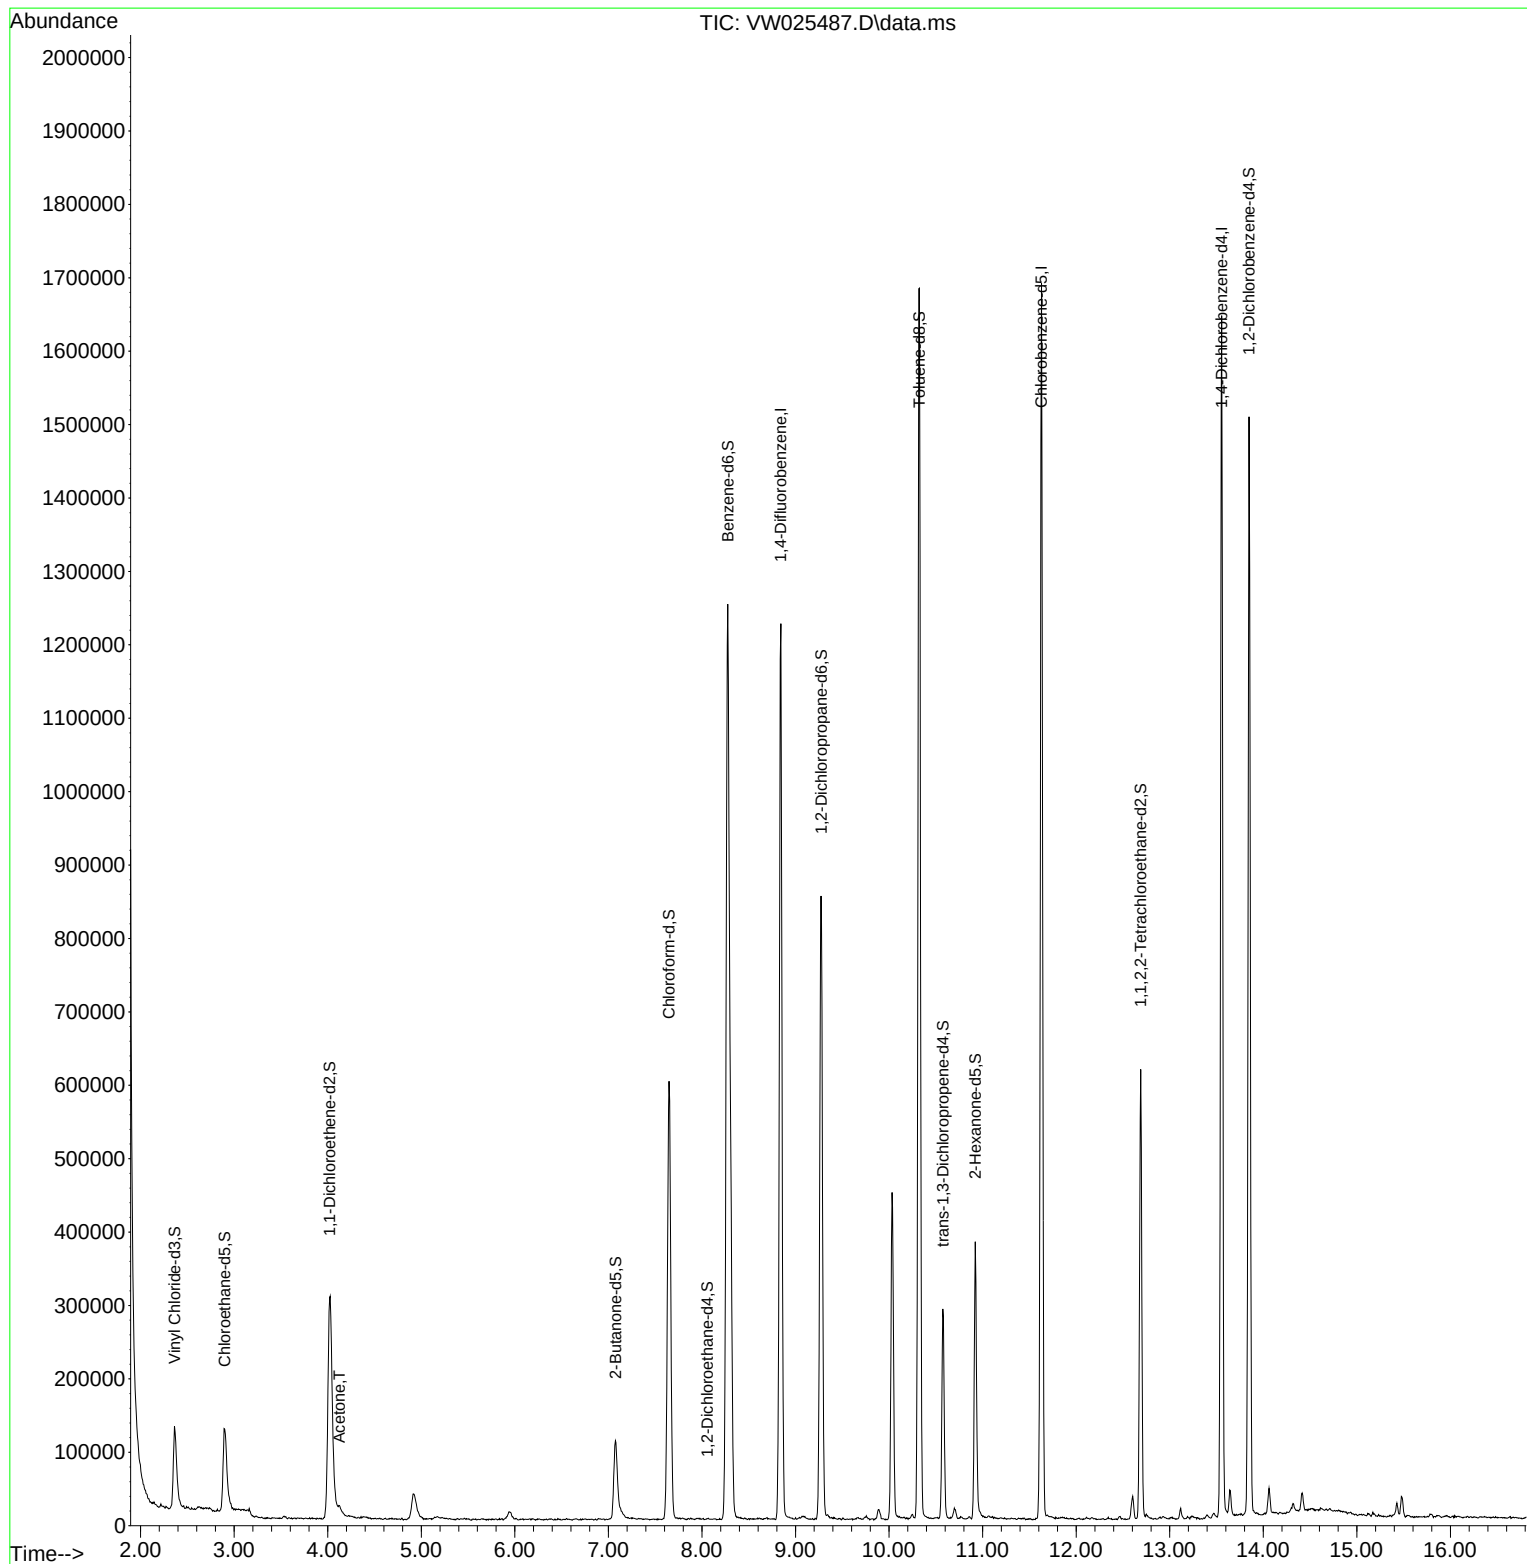

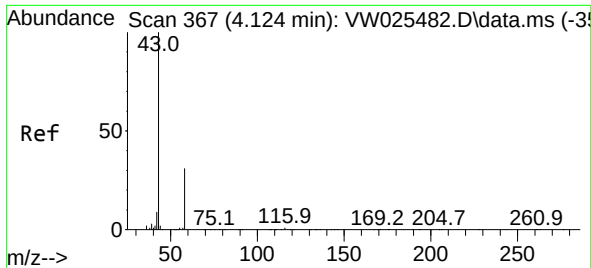

#13
 Acetone
 Concen: 6.589 ug/L
 RT: 4.124 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW025487.D
 Acq: 29 Mar 2023 15:19

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 43 Resp: 24704
 Ion Ratio Lower Upper
 43 100
 58 29.1 0.0 60.0

