


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW033119\
Data File : VW009604.D
Acq On : 31 Mar 2019 10:30
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5.0ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W032919S.M
Title : SW846 8260
Last Update : Fri Mar 29 13:24:53 2019

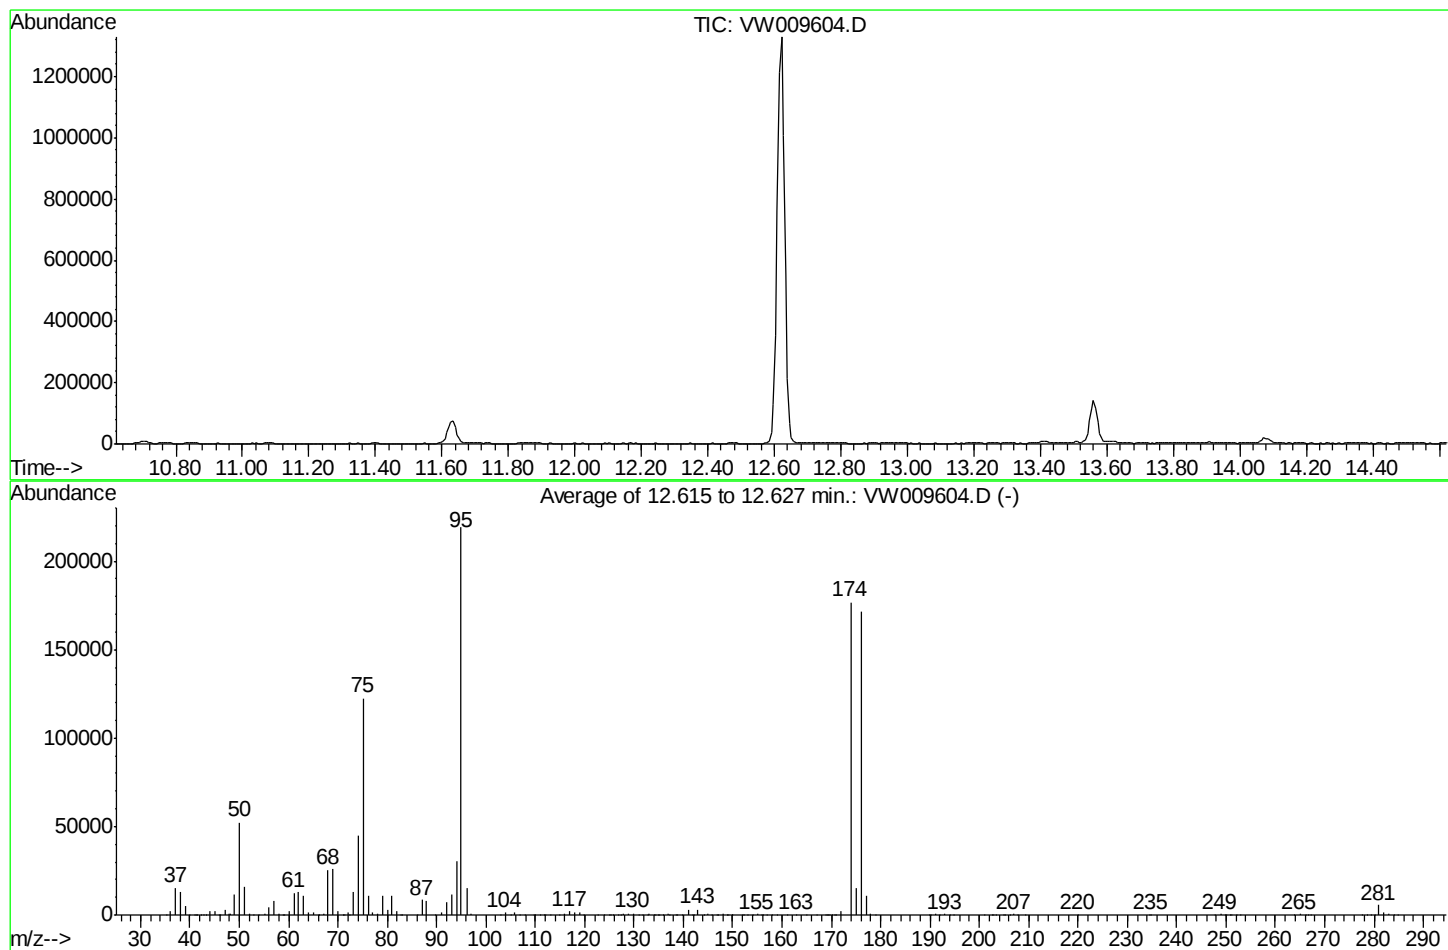

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.9	52434	PASS
75	95	30	60	55.9	122589	PASS
95	95	100	100	100.0	219178	PASS
96	95	5	9	7.0	15308	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	80.6	176640	PASS
175	174	5	9	8.7	15440	PASS
176	174	95	101	97.0	171349	PASS
177	176	5	9	6.5	11148	PASS