

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022367.D
 Acq On : 01 Apr 2022 15:31
 Operator : SY/VA
 Sample : VW0401SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK471

Quant Time: Apr 02 02:35:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	264702	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	254659	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	131654	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	97768	22.537	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	90.160%		
7) Chloroethane-d5	2.891	69	63230	24.415	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	97.640%		
11) 1,1-Dichloroethene-d2	4.025	63	118799	18.456	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	73.840%		
21) 2-Butanone-d5	7.080	46	54227	51.156	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	102.320%		
24) Chloroform-d	7.653	84	180836	24.501	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	98.000%		
26) 1,2-Dichloroethane-d4	8.305	65	115862	26.548	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	106.200%		
32) Benzene-d6	8.275	84	370920	26.524	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	106.080%		
36) 1,2-Dichloropropane-d6	9.274	67	110550	26.332	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	105.320%		
41) Toluene-d8	10.323	98	350649	26.356	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	105.440%		
43) trans-1,3-Dichloroprop...	10.579	79	53864	25.513	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	102.040%		
47) 2-Hexanone-d5	10.920	63	45913	53.387	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	106.780%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	89250	25.199	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	100.800%		
66) 1,2-Dichlorobenzene-d4	13.853	152	113702	26.753	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	107.000%		
Target Compounds					Qvalue	
48) 2-Hexanone	10.920	43	6008	2.988	ug/L	# 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
Data File : VW022367.D
Acq On : 01 Apr 2022 15:31
Operator : SY/VA
Sample : VW0401SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK471

Quant Time: Apr 02 02:35:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 02 02:06:11 2022
Response via : Initial Calibration

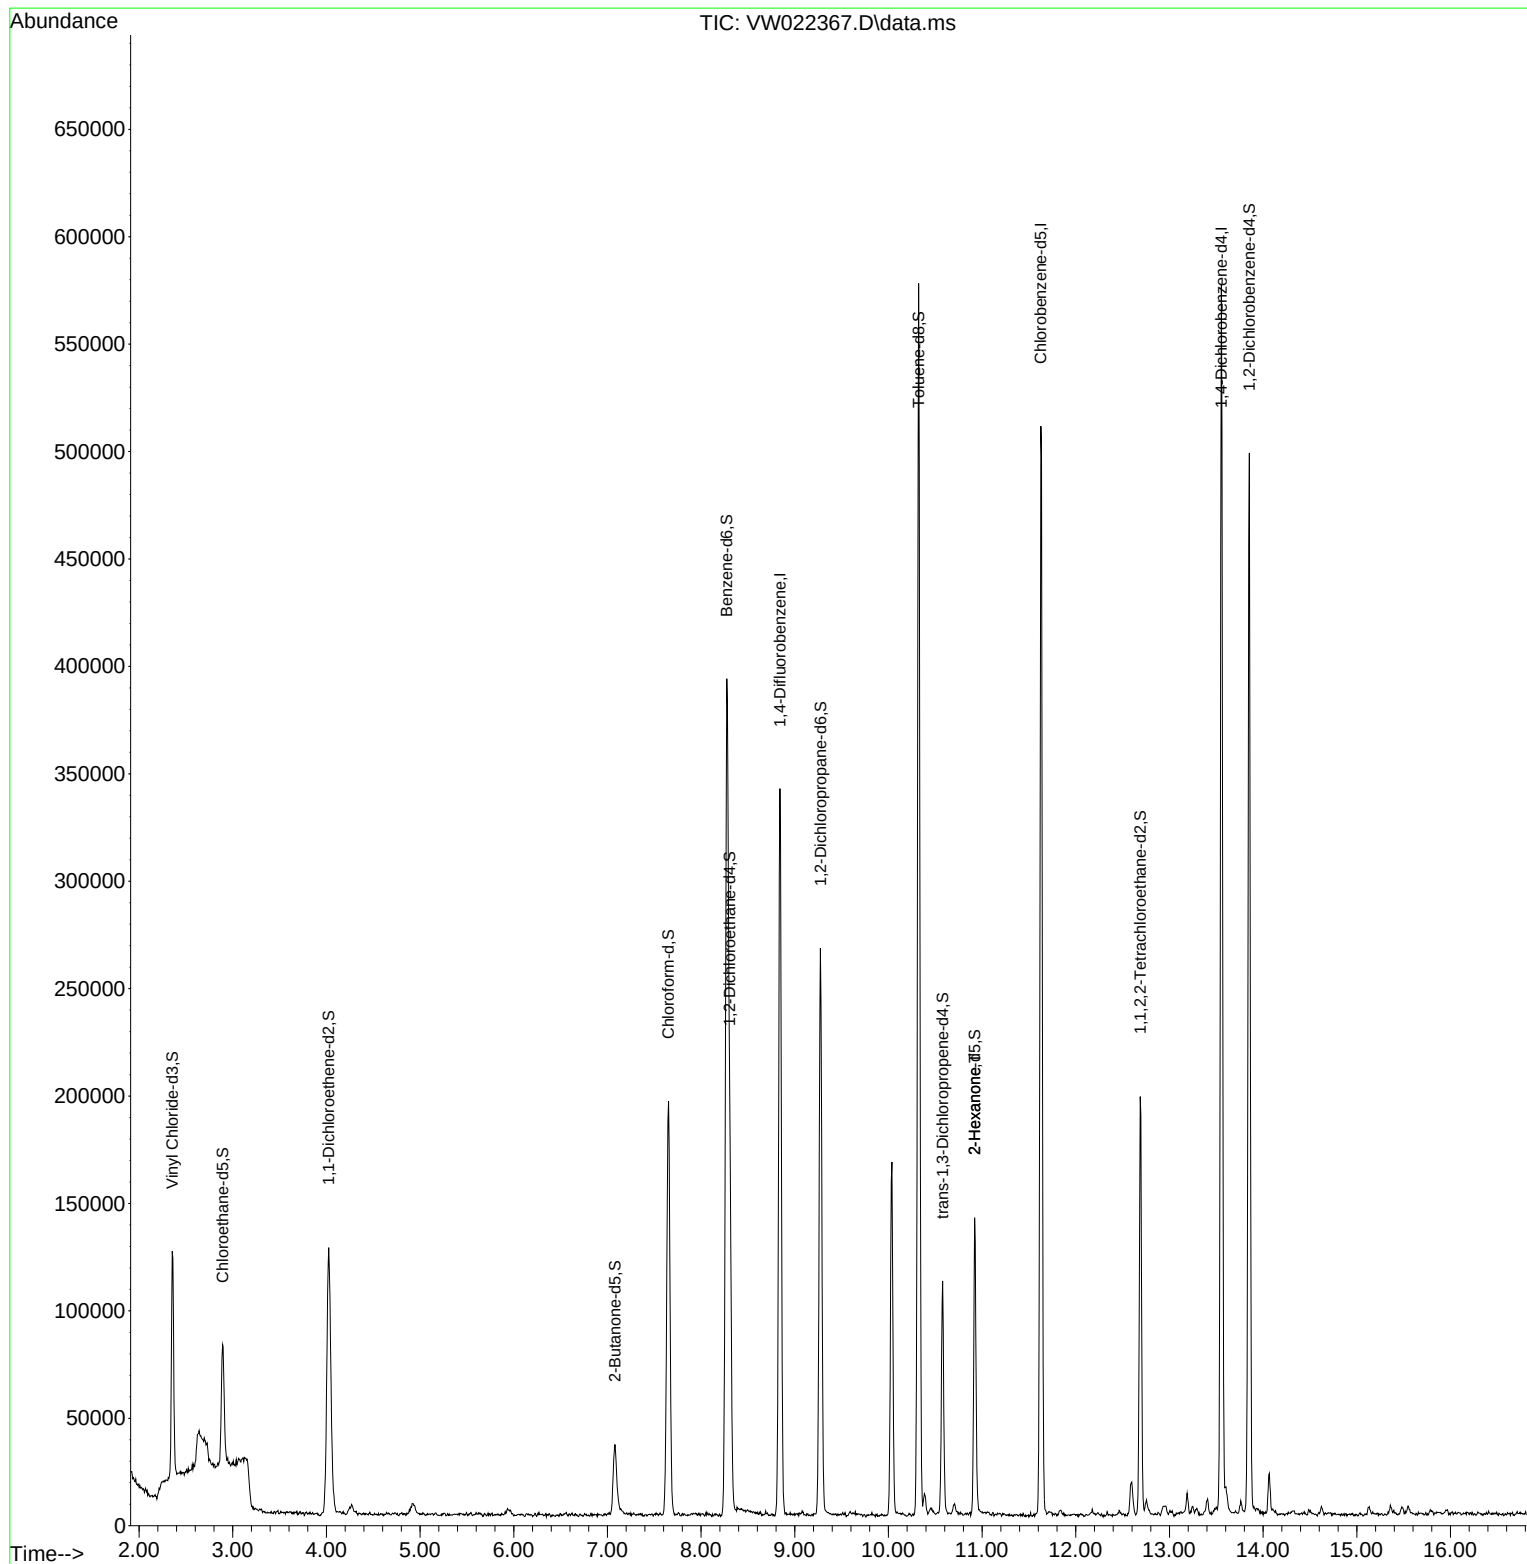

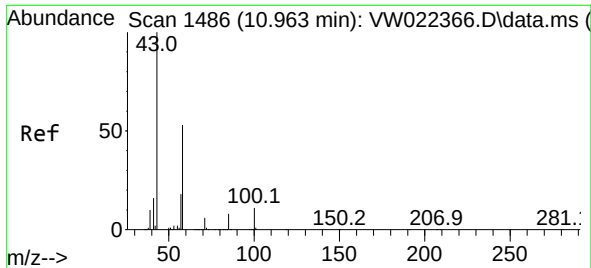

#48

2-Hexanone

Concen: 2.988 ug/L

RT: 10.920 min Scan# 14

Delta R.T. -0.043 min

Lab File: VW022367.D


Acq: 01 Apr 2022 15:31

Instrument :

MSVOA_W

ClientSampleId :

VBLK471

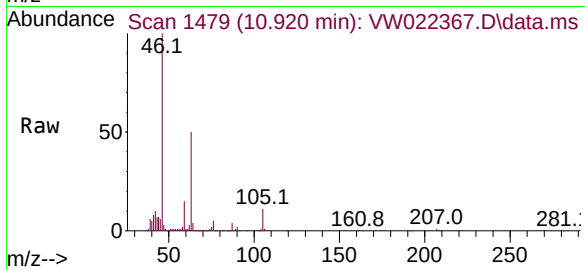

Tgt Ion: 43 Resp: 6008

Ion Ratio Lower Upper

43 100

58 28.2 44.6 66.8#

57 25.1 15.8 23.8#

100 0.0 12.7 19.1#

