

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022372.D
 Acq On : 01 Apr 2022 17:31
 Operator : SY/VA
 Sample : N2225-05
 Misc : 7.88g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQD4

Quant Time: Apr 02 02:36:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.842	114	222068	25.000	ug/L	# 0.00
28) Chlorobenzene-d5		11.628	117	219328	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.554	152	112915	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.355	65	106415	29.239	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	116.960%	
7) Chloroethane-d5		2.892	69	60865	28.013	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	112.040%	
11) 1,1-Dichloroethene-d2		4.026	63	101553	18.806	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.240%	
21) 2-Butanone-d5		7.074	46	87408	98.288	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	196.580%#	
24) Chloroform-d		7.653	84	164929	26.636	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	106.560%	
26) 1,2-Dichloroethane-d4		8.397	65	229	0.063	ug/L	0.09
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.240%#	
32) Benzene-d6		8.275	84	336057	27.902	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	111.600%	
36) 1,2-Dichloropropane-d6		9.275	67	104680	28.950	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	115.800%	
41) Toluene-d8		10.323	98	326397	28.485	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	113.920%	
43) trans-1,3-Dichloroprop...		10.579	79	56400	31.018	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	124.080%	
47) 2-Hexanone-d5		10.921	63	70980	95.829	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	191.660%#	
56) 1,1,2,2-Tetrachloroeth...		12.689	84	115147	37.748	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	151.000%#	
66) 1,2-Dichlorobenzene-d4		13.853	152	104176	28.580	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	114.320%	
Target Compounds							Qvalue
42) Toluene		10.384	91	14785	0.944	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
Data File : VW022372.D
Acq On : 01 Apr 2022 17:31
Operator : SY/VA
Sample : N2225-05
Misc : 7.88g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGQD4

Quant Time: Apr 02 02:36:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 02 02:06:11 2022
Response via : Initial Calibration

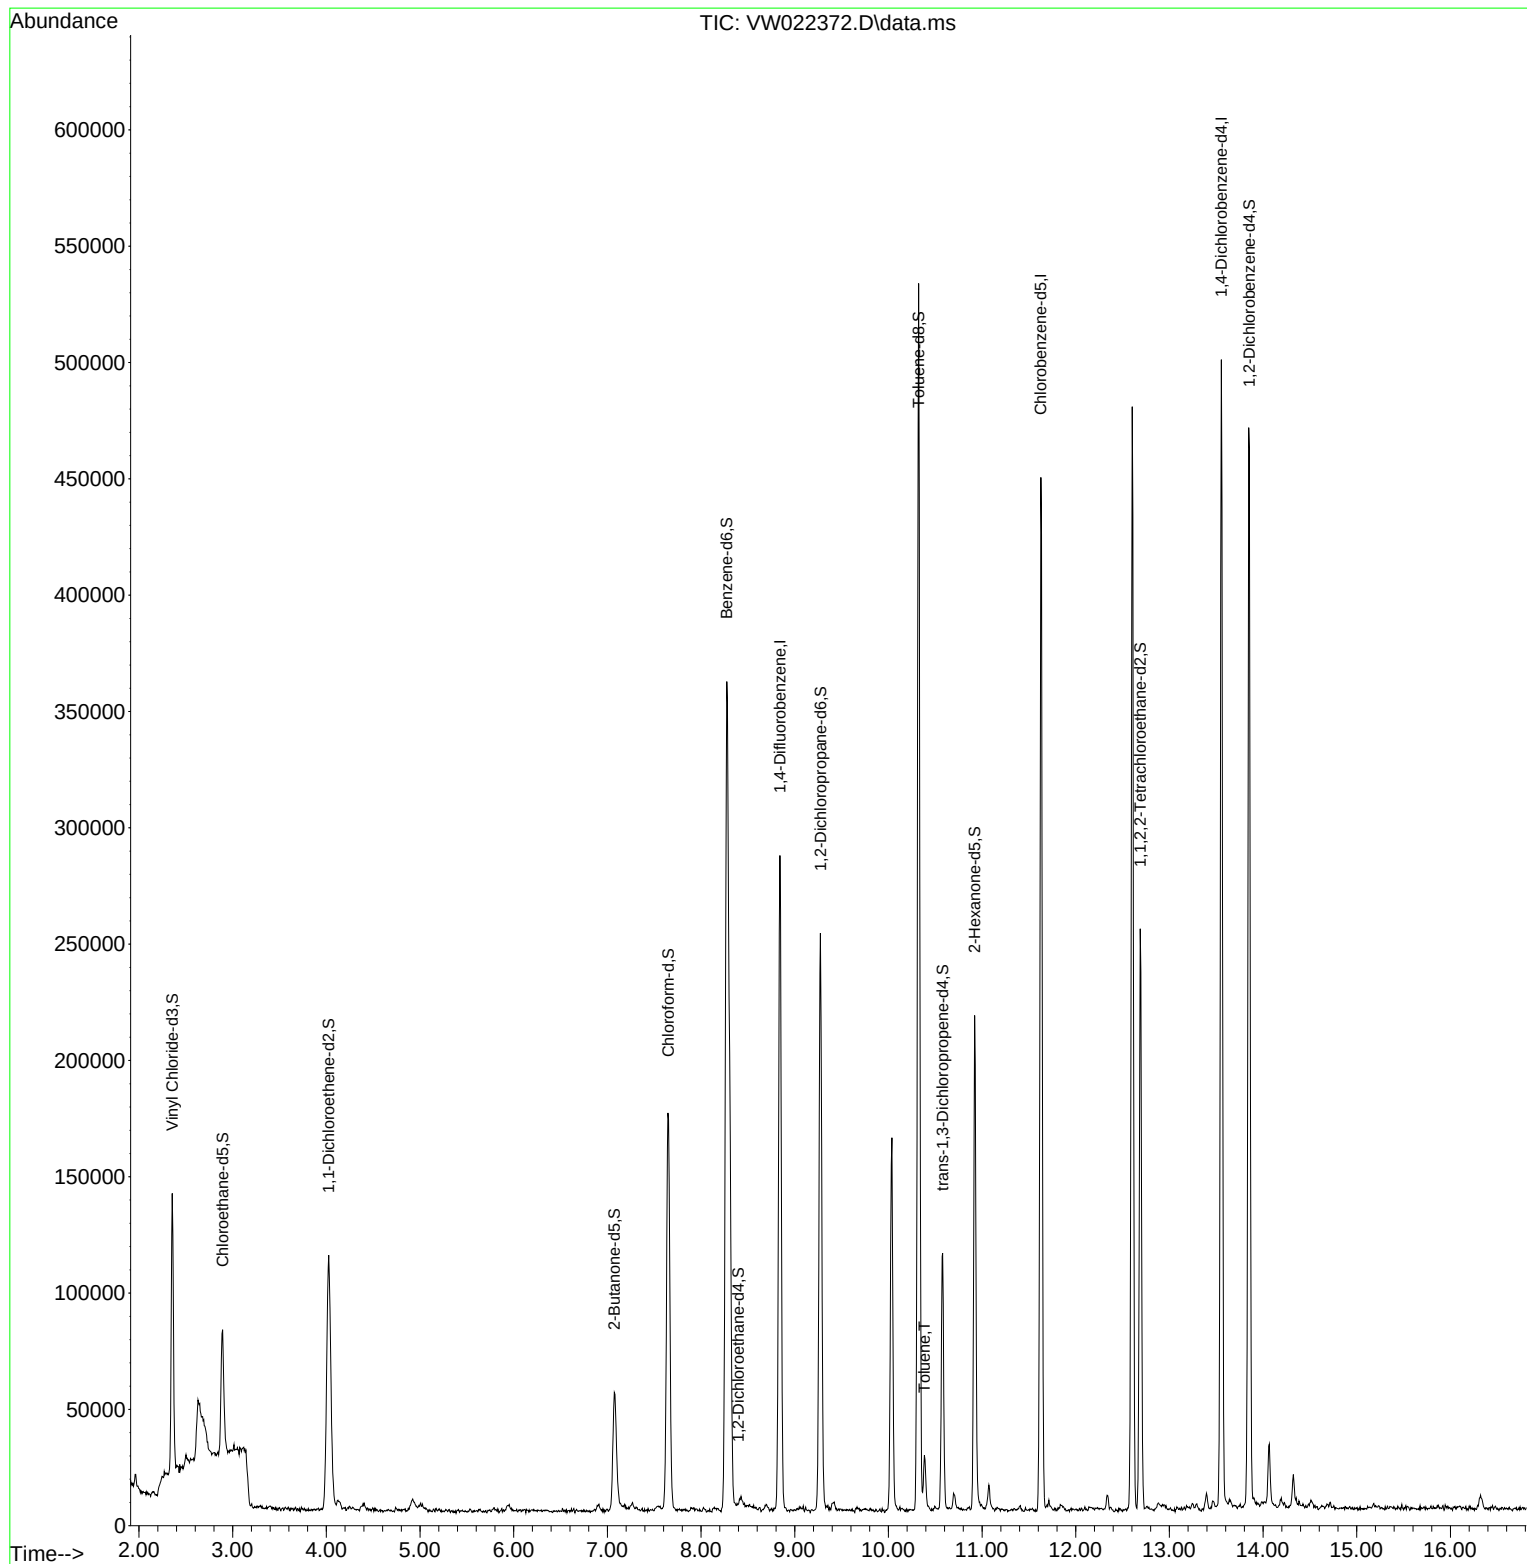

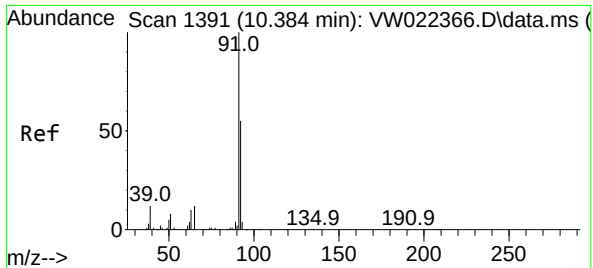

#42
Toluene
Concen: 0.944 ug/L
RT: 10.384 min Scan# 11
Delta R.T. 0.000 min
Lab File: VW022372.D
Acq: 01 Apr 2022 17:31

Instrument :
MSVOA_W
ClientSampleId :
BGQD4

Tgt Ion: 91 Resp: 14785
Ion Ratio Lower Upper
91 100
92 60.7 40.4 75.0

