

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022373.D
 Acq On : 01 Apr 2022 17:55
 Operator : SY/VA
 Sample : N2225-06
 Misc : 7.48g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQD5

Quant Time: Apr 02 02:36:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.841	114	308815	25.000	ug/L	# 0.00
28) Chlorobenzene-d5		11.628	117	294910	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.554	152	145960	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.355	65	127011	25.095	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 100.400%		
7) Chloroethane-d5		2.885	69	73388	24.289	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 97.160%		
11) 1,1-Dichloroethene-d2		4.019	63	120662	16.068	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	= 64.280%		
21) 2-Butanone-d5		7.074	46	65285	52.790	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 105.580%		
24) Chloroform-d		7.647	84	196351	22.803	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	= 91.200%		
26) 1,2-Dichloroethane-d4		8.433	65	105	0.021	ug/L	0.13
Spiked Amount	25.000	Range	70 - 130	Recovery	= 0.080%#		
32) Benzene-d6		8.275	84	408042	25.196	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	= 100.800%		
36) 1,2-Dichloropropane-d6		9.274	67	122153	25.124	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	= 100.480%		
41) Toluene-d8		10.445	98	140	0.009	ug/L	0.12
Spiked Amount	25.000	Range	30 - 130	Recovery	= 0.040%#		
43) trans-1,3-Dichloroprop...		10.579	79	60179	24.614	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	= 98.440%		
47) 2-Hexanone-d5		10.920	63	53969	54.189	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 108.380%		
56) 1,1,2,2-Tetrachloroeth...		12.688	84	103854	25.320	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	= 101.280%		
66) 1,2-Dichlorobenzene-d4		13.853	152	118424	25.133	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	= 100.520%		
Target Compounds							
13) Acetone		4.141	43	2645	3.123	ug/L	81
42) Toluene		10.390	91	21475	1.020	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
Data File : VW022373.D
Acq On : 01 Apr 2022 17:55
Operator : SY/VA
Sample : N2225-06
Misc : 7.48g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGQD5

Quant Time: Apr 02 02:36:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 02 02:06:11 2022
Response via : Initial Calibration

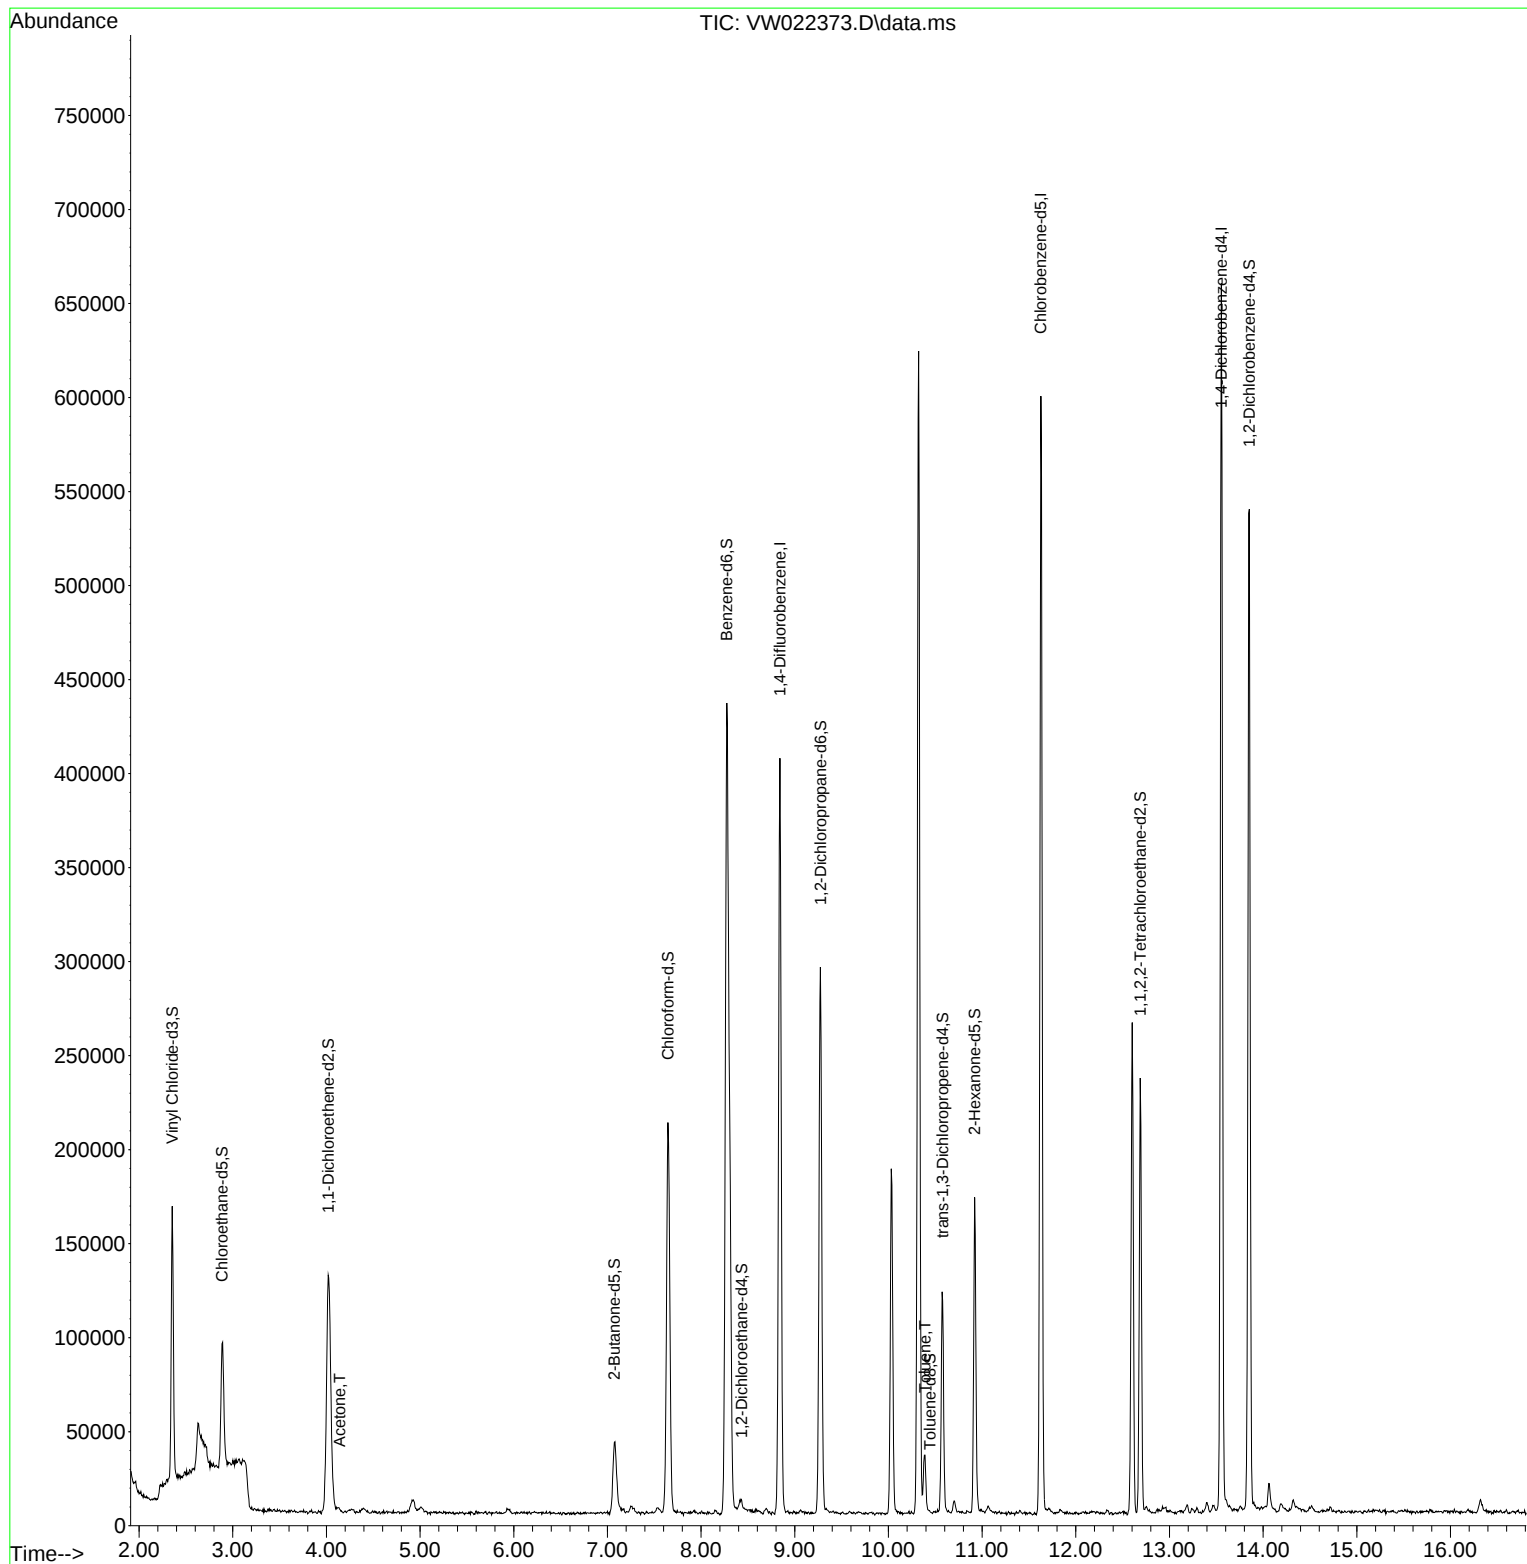

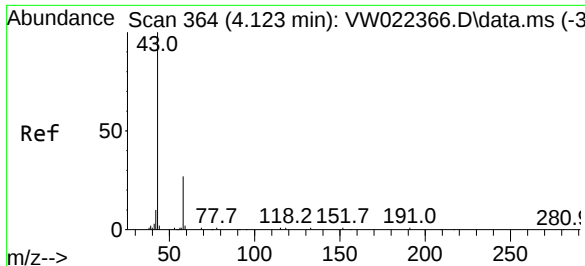

#13

Acetone

Concen: 3.123 ug/L

RT: 4.141 min Scan# 3

Delta R.T. 0.018 min

Lab File: VW022373.D

Acq: 01 Apr 2022 17:55

Instrument :

MSVOA_W

ClientSampleId :





BGQD5

Tgt Ion: 43 Resp: 2645

Ion Ratio Lower Upper

43 100

58 23.9 0.0 69.2

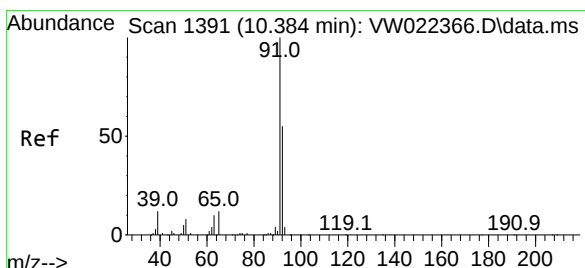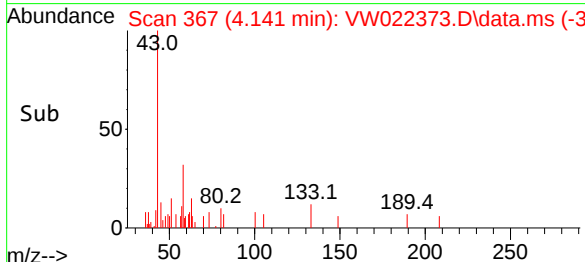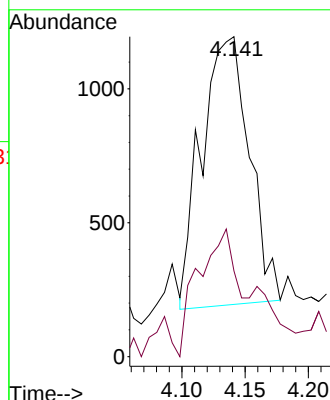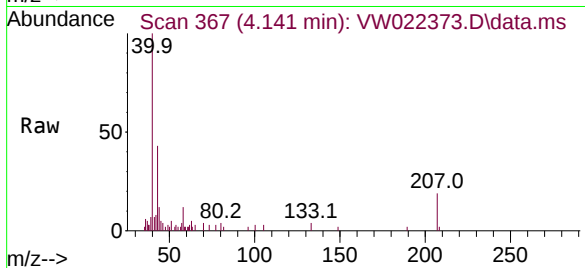

#42

Toluene

Concen: 1.020 ug/L

RT: 10.390 min Scan# 1392

Delta R.T. 0.006 min

Lab File: VW022373.D

Acq: 01 Apr 2022 17:55

Tgt Ion: 91 Resp: 21475

Ion Ratio Lower Upper

91 100

92 56.7 40.4 75.0

