

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022375.D
 Acq On : 01 Apr 2022 18:43
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK408

Quant Time: Apr 02 02:36:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	234535	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	232422	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	114643	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	121291	31.555	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 126.200%	
7) Chloroethane-d5	2.885	69	69332	30.214	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 120.840%	
11) 1,1-Dichloroethene-d2	4.019	63	113062	19.824	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	= 79.280%	
21) 2-Butanone-d5	7.080	46	55489	59.079	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 118.160%	
24) Chloroform-d	7.653	84	186517	28.522	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	= 114.080%	
26) 1,2-Dichloroethane-d4	8.305	65	122067	31.567	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	= 126.280%	
32) Benzene-d6	8.275	84	389990	30.556	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	= 122.240%	
36) 1,2-Dichloropropane-d6	9.274	67	115170	30.057	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	= 120.240%#	
41) Toluene-d8	10.323	98	378144	31.142	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	= 124.560%	
43) trans-1,3-Dichloroprop...	10.573	79	55295	28.697	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	= 114.800%	
47) 2-Hexanone-d5	10.920	63	46170	58.822	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 117.640%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	93945	29.062	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	= 116.240%	
66) 1,2-Dichlorobenzene-d4	13.847	152	117783	31.826	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	= 127.320%#	
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.030	75	5451	0.902	ug/L	# 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
Data File : VW022375.D
Acq On : 01 Apr 2022 18:43
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK408

Quant Time: Apr 02 02:36:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 02 02:06:11 2022
Response via : Initial Calibration

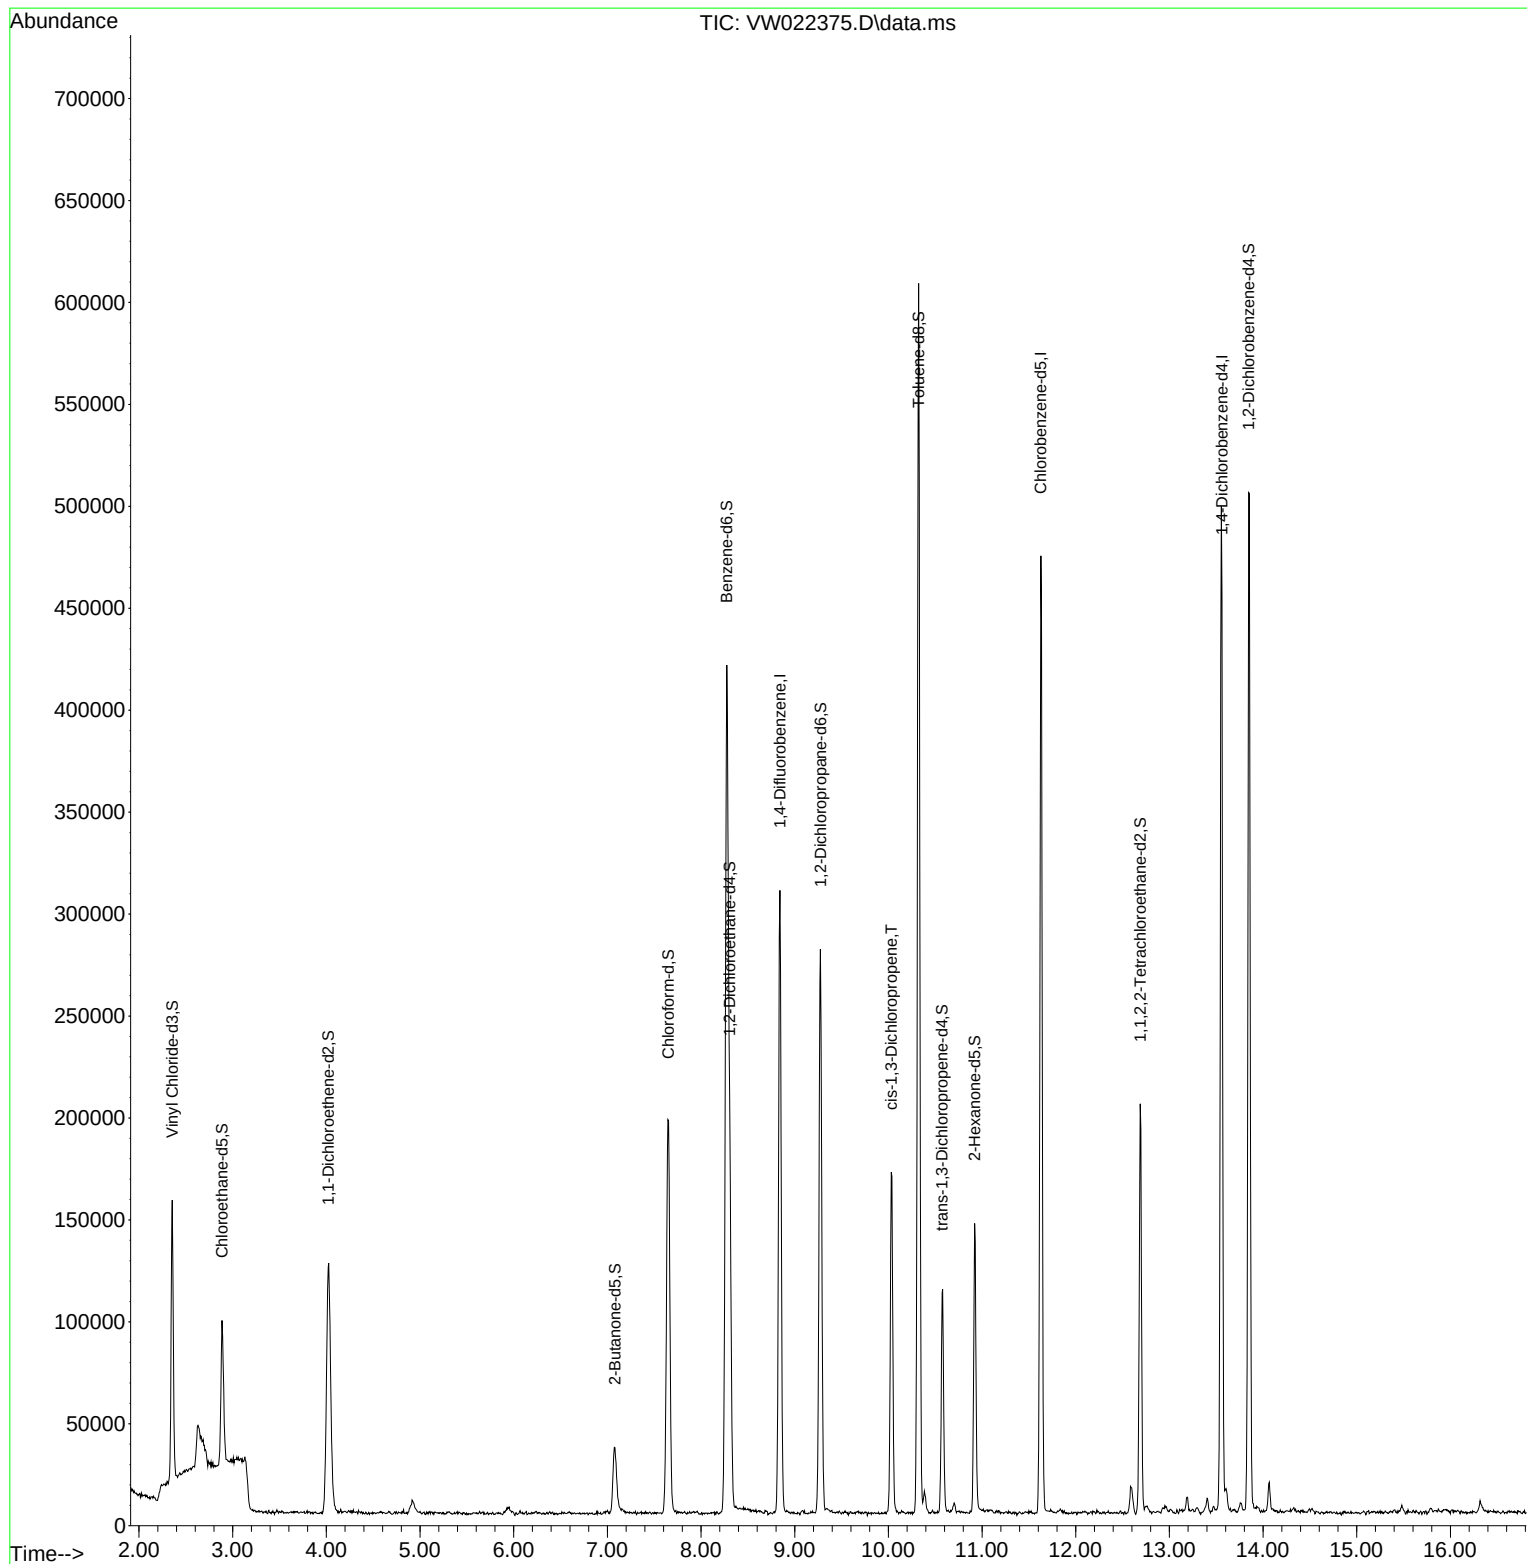

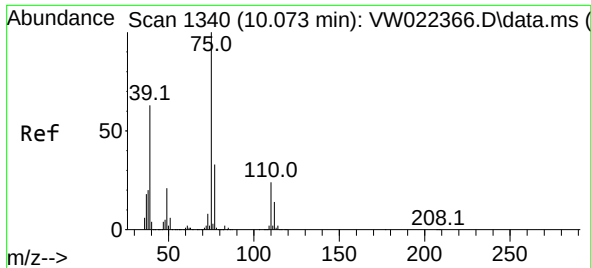

#39
 cis-1,3-Dichloropropene
 Concen: 0.902 ug/L
 RT: 10.030 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VW022375.D
 Acq: 01 Apr 2022 18:43

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK408

Tgt Ion: 75 Resp: 5451
 Ion Ratio Lower Upper
 75 100
 77 39.0 20.6 38.2#

