
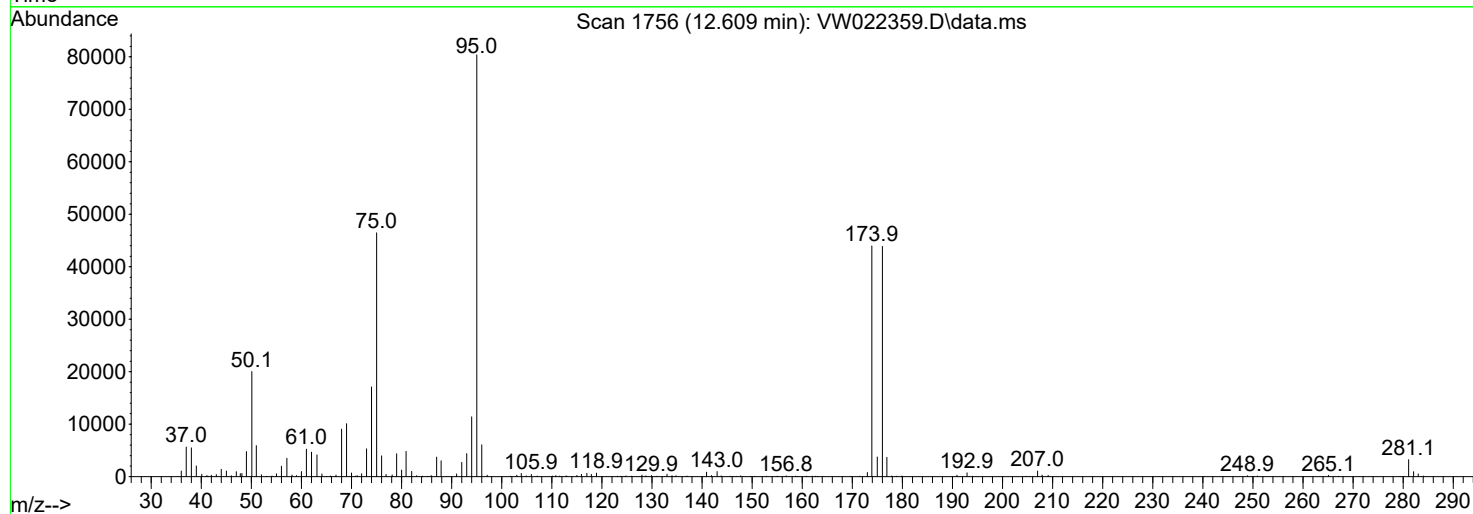


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
Data File : VW022359.D
Acq On : 01 Apr 2022 10:37
Operator : SY/VA
Sample : BFB
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB525

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Title : SFAM01.0
Last Update : Sat Apr 02 02:06:11 2022

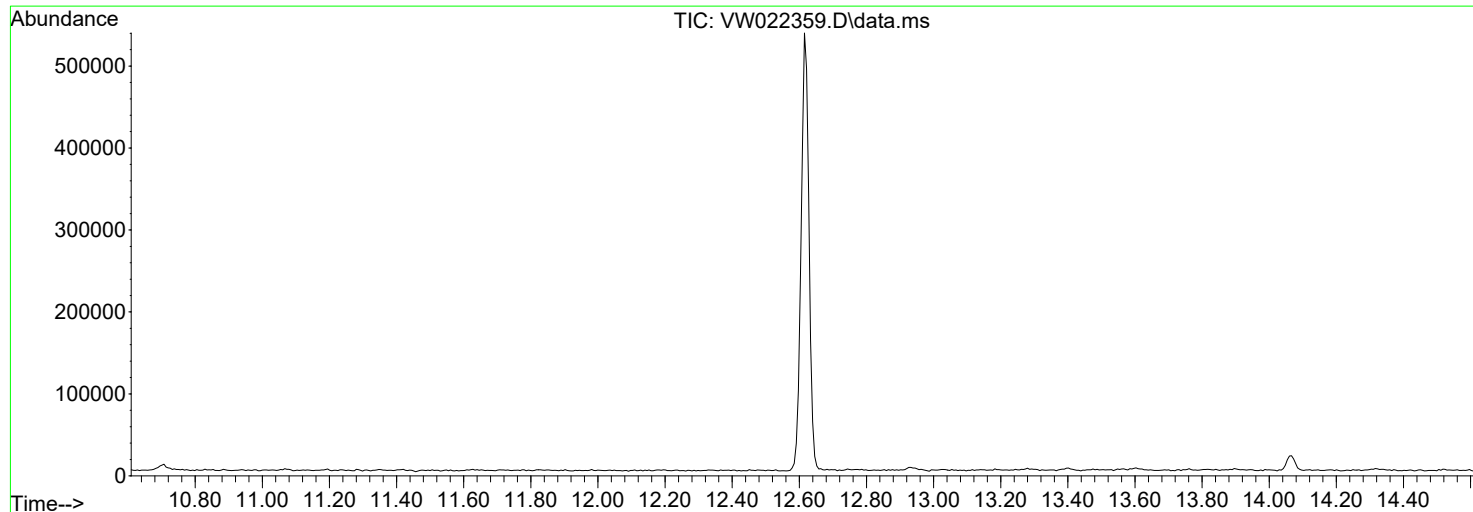

Spectrum Information: Scan 1756

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.9	20032	PASS
75	95	30	80	57.8	46464	PASS
95	95	100	100	100.0	80384	PASS
96	95	5	9	7.6	6082	PASS
173	174	0.00	2	1.8	791	PASS
174	95	50	120	54.7	43968	PASS
175	174	5	9	8.5	3753	PASS
176	174	95	105	99.8	43888	PASS
177	176	5	10	8.4	3683	PASS