




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022369.D
 Acq On : 01 Apr 2022 16:19
 Operator : SY/VA
 Sample : N2225-02
 Misc : 7.22g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQD1

Manual IntegrationsAPPROVED

Quant Time: Apr 02 02:35:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/02/2022
 Supervised By :Mahesh Dadoda 04/05/2022

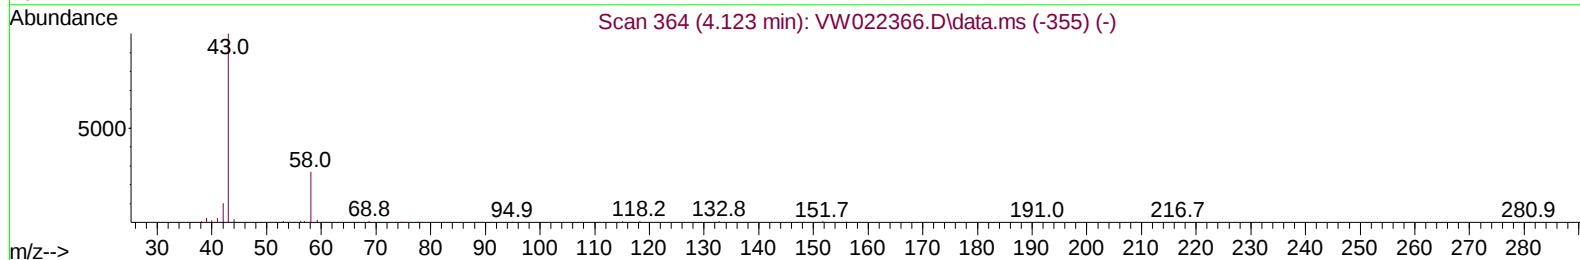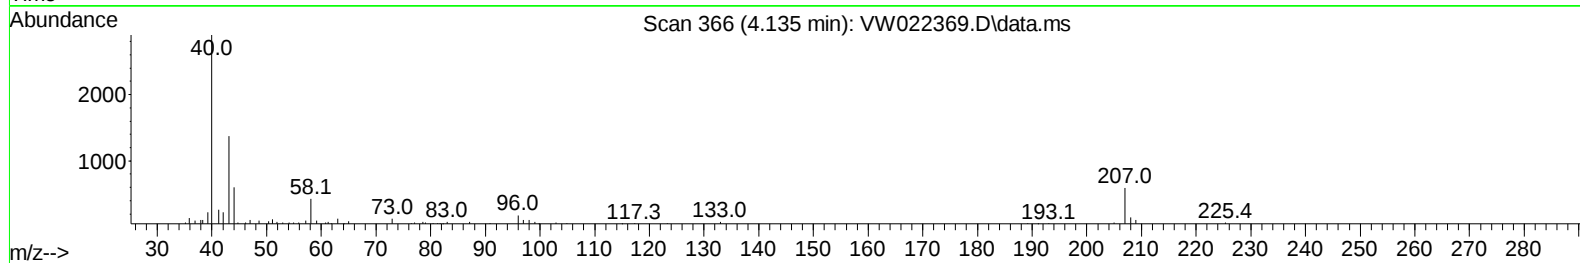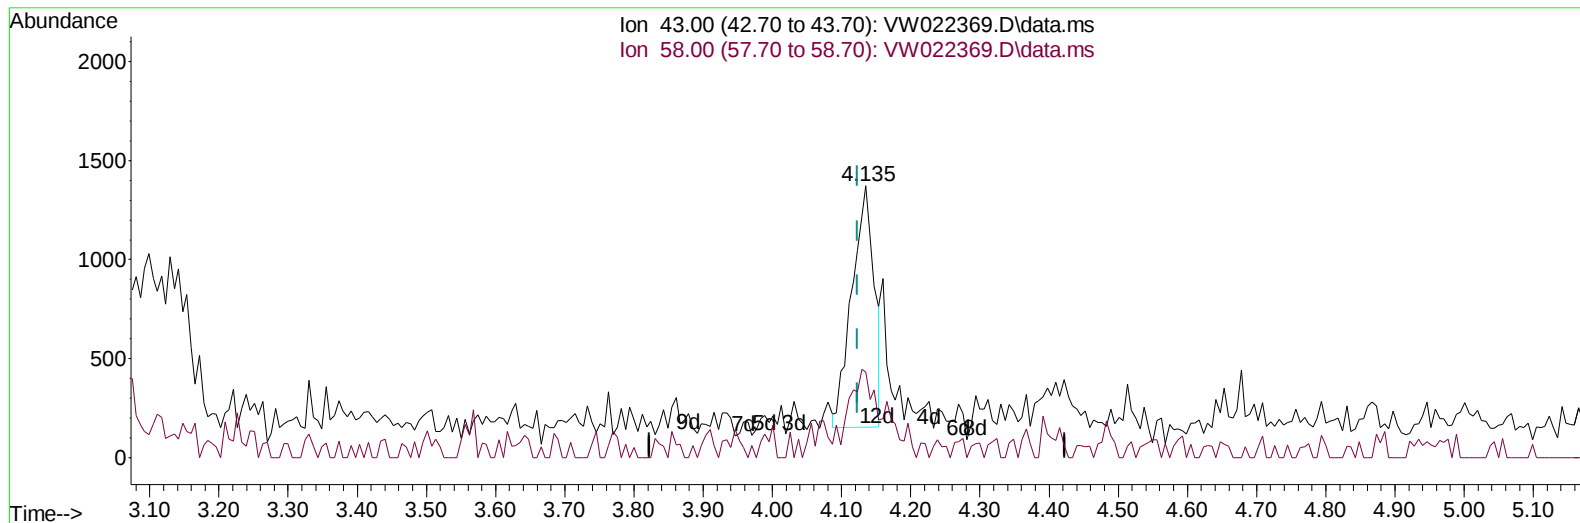

TIC: VW022369.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 3.88 ug/L

response 2738

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	18.52
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022369.D
 Acq On : 01 Apr 2022 16:19
 Operator : SY/VA
 Sample : N2225-02
 Misc : 7.22g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQD1

Manual IntegrationsAPPROVED

Quant Time: Apr 02 02:35:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/02/2022
 Supervised By :Mahesh Dadoda 04/05/2022

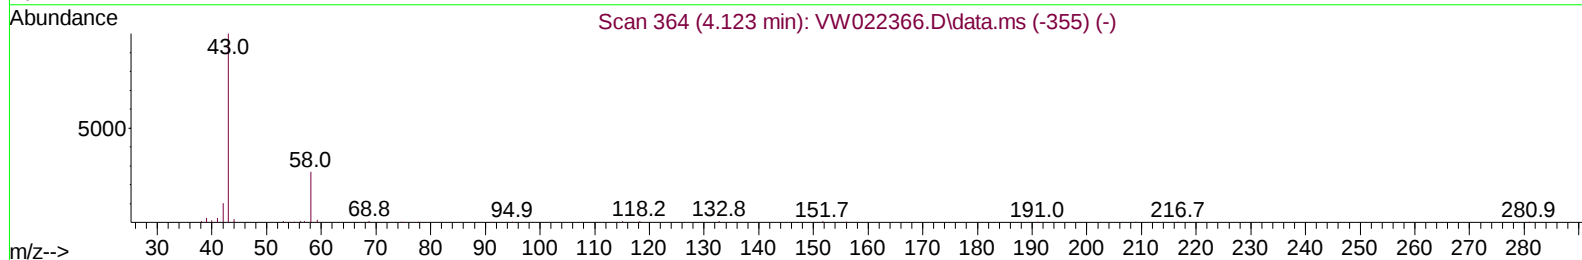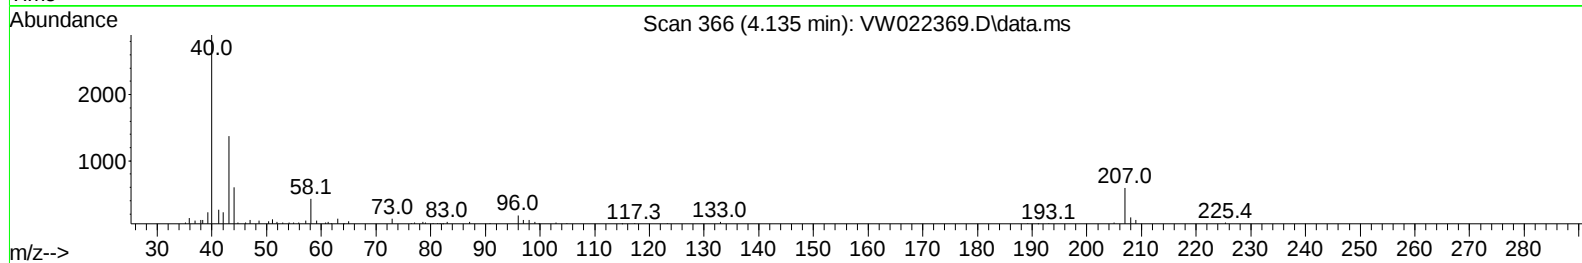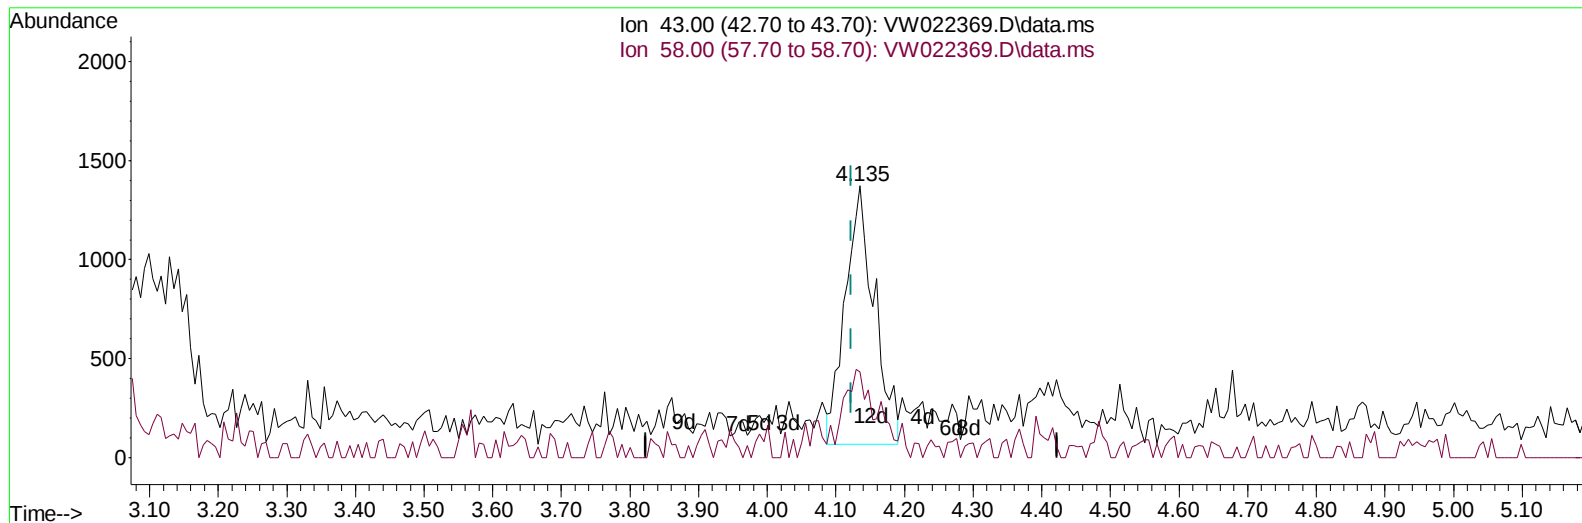

TIC: VW022369.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 5.49 ug/L m

response 3873

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	13.09
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022369.D
 Acq On : 01 Apr 2022 16:19
 Operator : SY/VA
 Sample : N2225-02
 Misc : 7.22g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQD1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/02/2022
 Supervised By :Mahesh Dadoda 04/05/2022

Quant Time: Apr 02 02:35:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

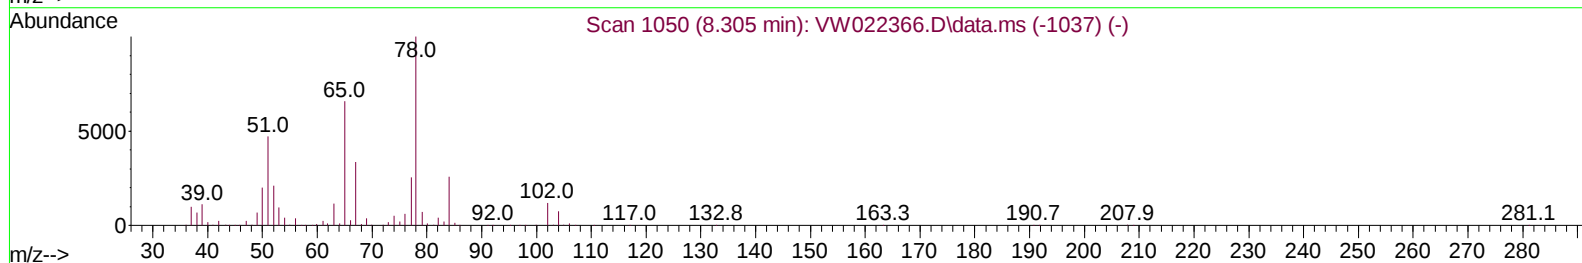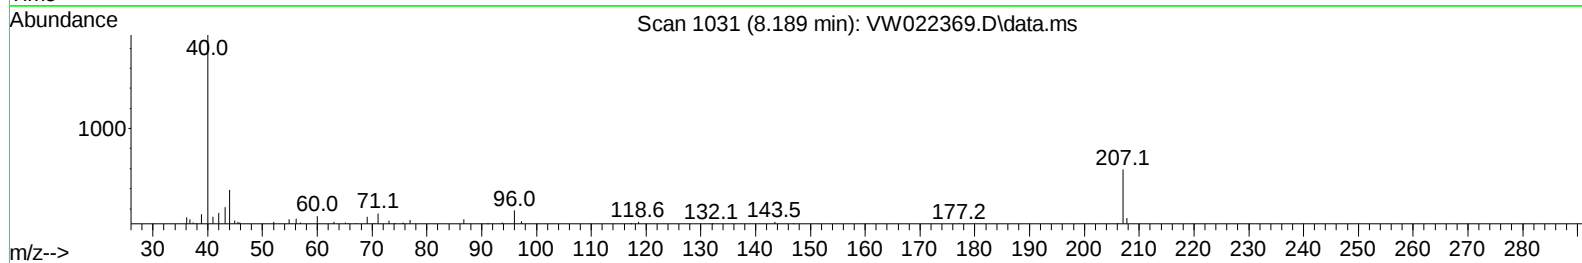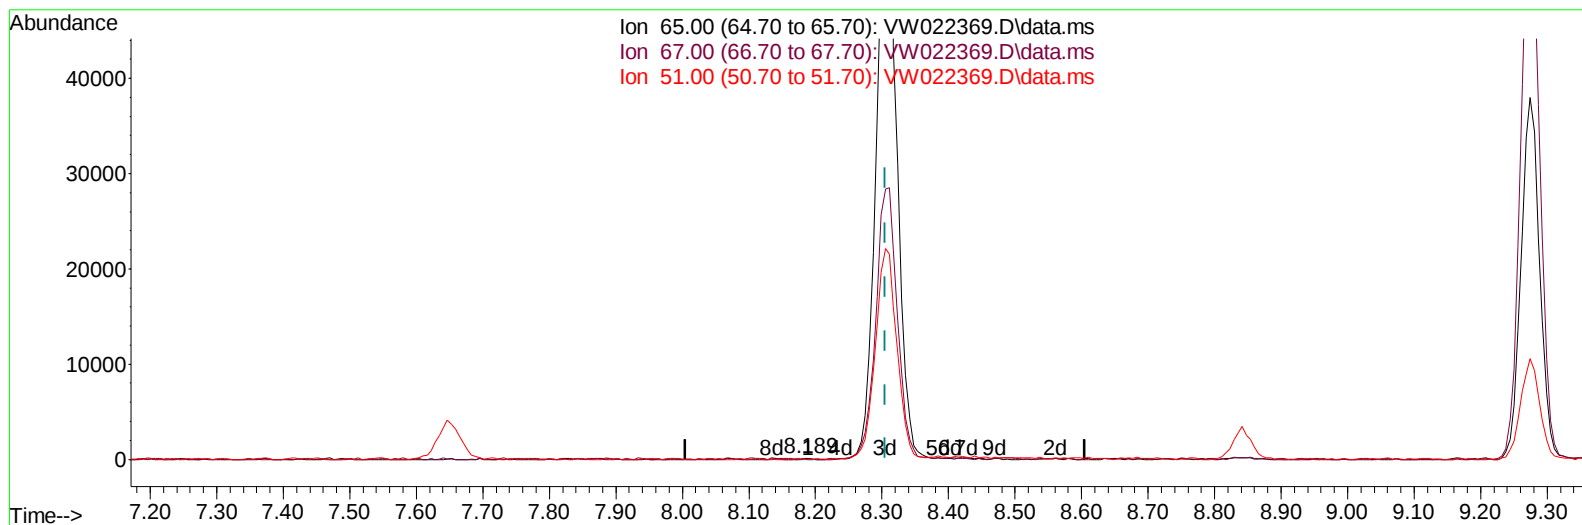

TIC: VW022369.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.189min (-0.116) 0.03 ug/L

response 114

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.50	62.28
51.00	90.00	71.93
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022369.D
 Acq On : 01 Apr 2022 16:19
 Operator : SY/VA
 Sample : N2225-02
 Misc : 7.22g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQD1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/02/2022
 Supervised By :Mahesh Dadoda 04/05/2022

Quant Time: Apr 02 02:35:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

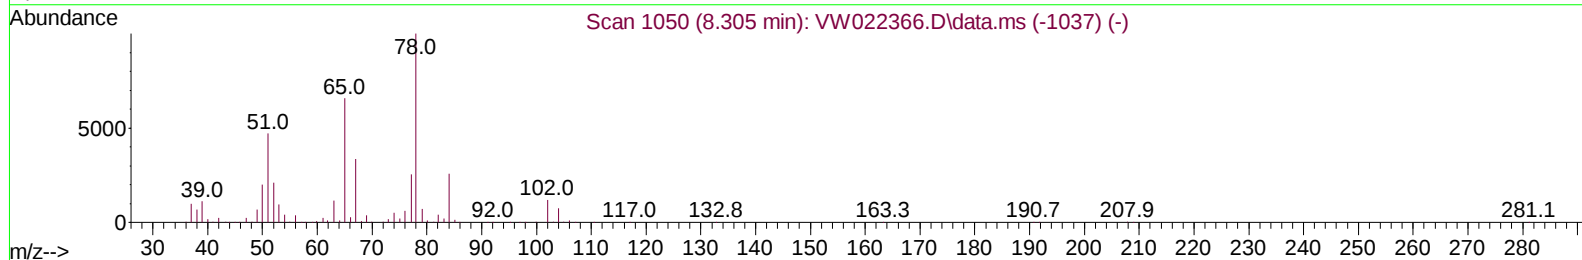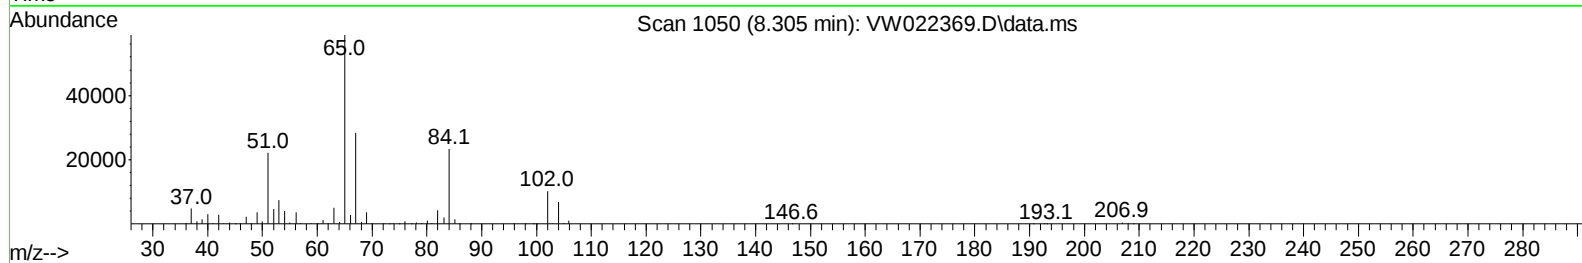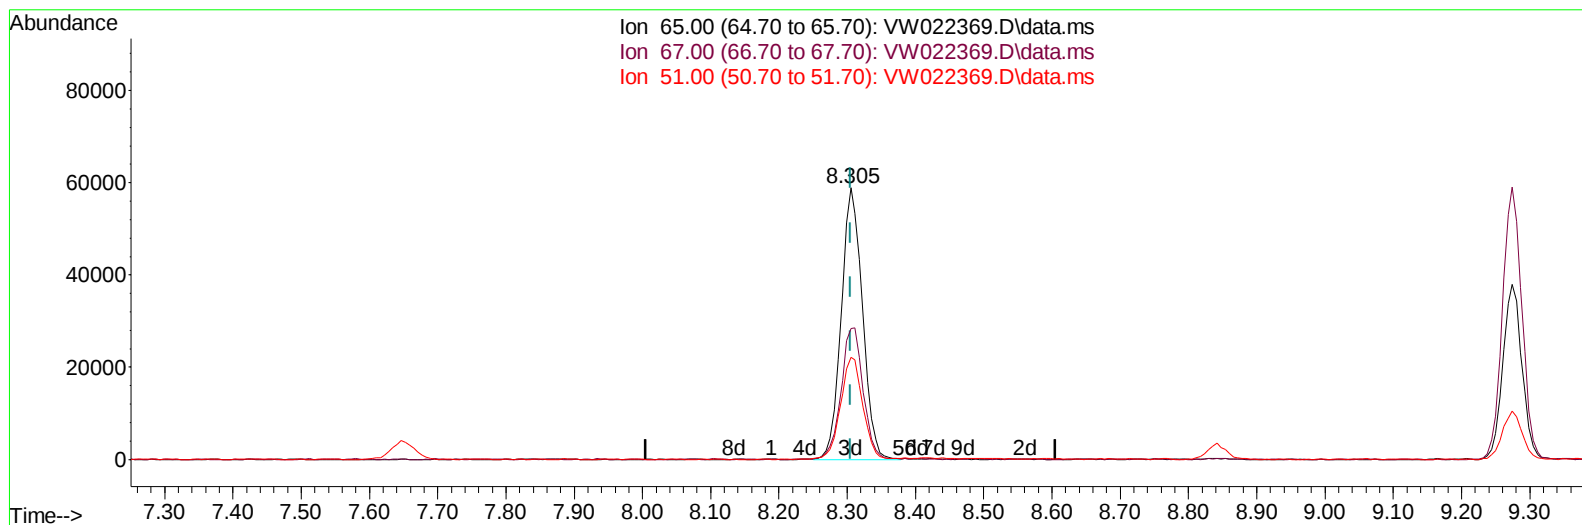

TIC: VW022369.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 29.97 ug/L m

response 127034

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.50	0.06#
51.00	90.00	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022369.D
 Acq On : 01 Apr 2022 16:19
 Operator : SY/VA
 Sample : N2225-02
 Misc : 7.22g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQD1

Manual IntegrationsAPPROVED

Quant Time: Apr 02 02:35:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/02/2022
 Supervised By :Mahesh Dadoda 04/05/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		257098	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117		249135	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		124076	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		122897	29.167	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	116.680%	
7) Chloroethane-d5	2.892	69		67132	26.688	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	106.760%	
11) 1,1-Dichloroethene-d2	4.019	63		120497	19.274	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110		Recovery	=	77.080%	
21) 2-Butanone-d5	7.080	46		78897	76.630	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	153.260%#	
24) Chloroform-d	7.653	84		185062	25.816	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	103.280%	
26) 1,2-Dichloroethane-d4	8.305	65		127034m	29.969	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	119.880%	
32) Benzene-d6	8.275	84		385437	28.173	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	112.680%	
36) 1,2-Dichloropropane-d6	9.274	67		116610	28.391	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	113.560%	
41) Toluene-d8	10.323	98		363369	27.918	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	111.680%	
43) trans-1,3-Dichloroprop...	10.579	79		60158	29.127	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	116.520%	
47) 2-Hexanone-d5	10.921	63		65312	77.627	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	155.260%#	
56) 1,1,2,2-Tetrachloroeth...	12.689	84		112929	32.592	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	130.360%#	
66) 1,2-Dichlorobenzene-d4	13.853	152		115994	28.959	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	115.840%	
Target Compounds							
13) Acetone	4.135	43		3873m	5.493	ug/L	Qvalue
42) Toluene	10.384	91		26553	1.493	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
Data File : VW022369.D
Acq On : 01 Apr 2022 16:19
Operator : SY/VA
Sample : N2225-02
Misc : 7.22g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGQD1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/02/2022
Supervised By :Mahesh Dadoda 04/05/2022

Quant Time: Apr 02 02:35:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 02 02:06:11 2022
Response via : Initial Calibration

