




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022372.D
 Acq On : 01 Apr 2022 17:31
 Operator : SY/VA
 Sample : N2225-05
 Misc : 7.88g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQD4

Manual IntegrationsAPPROVED

Quant Time: Apr 02 02:36:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/02/2022
 Supervised By :Mahesh Dadoda 04/05/2022

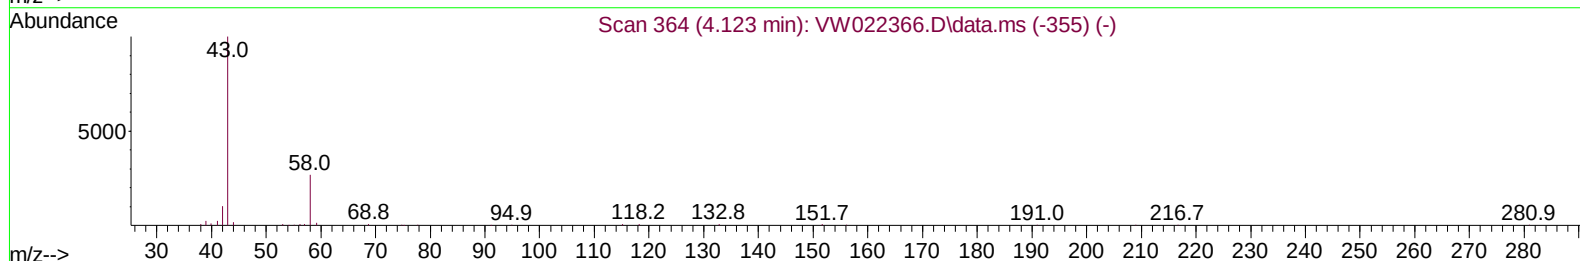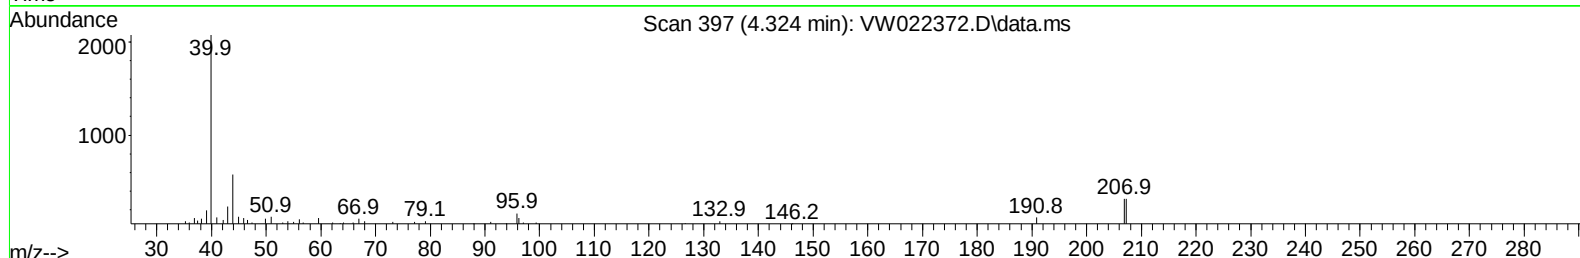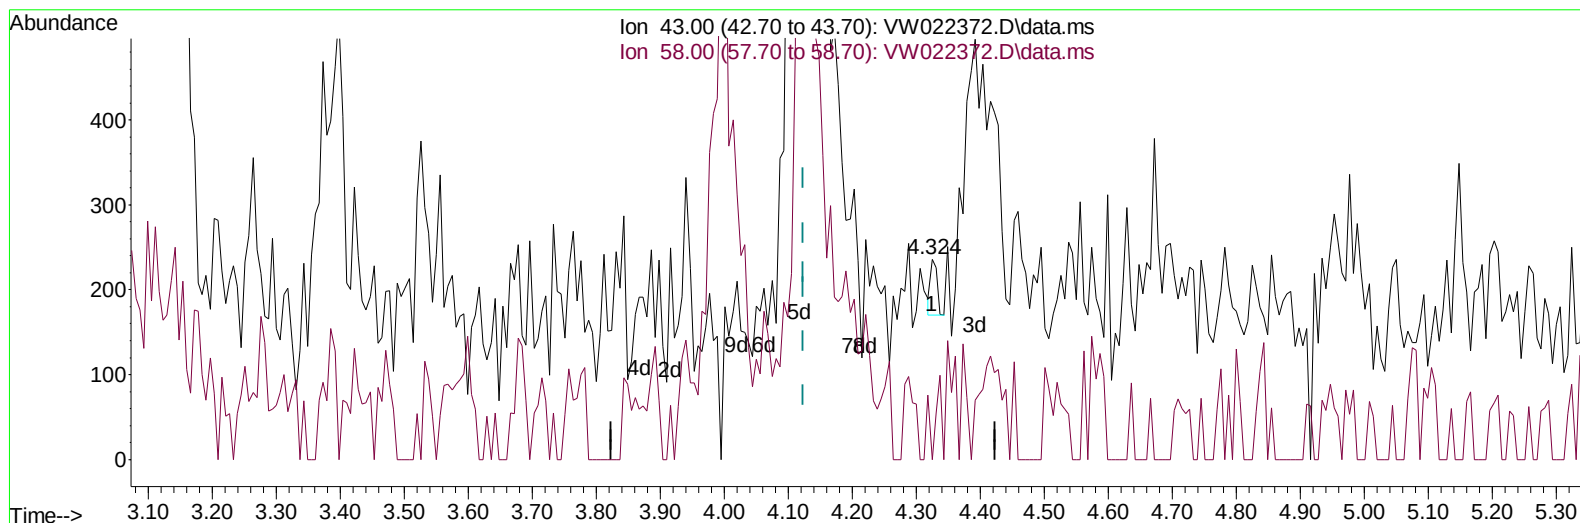

TIC: VW022372.D\data.ms

(13) Acetone (T)

4.324min (+ 0.201) 0.07 ug/L

response 45

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	62.22
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022372.D
 Acq On : 01 Apr 2022 17:31
 Operator : SY/VA
 Sample : N2225-05
 Misc : 7.88g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQD4

Manual IntegrationsAPPROVED

Quant Time: Apr 02 02:36:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/02/2022
 Supervised By :Mahesh Dadoda 04/05/2022

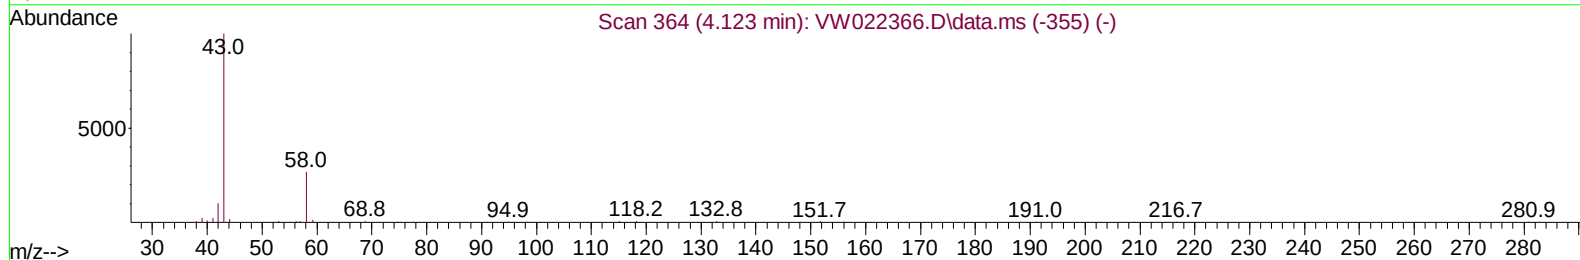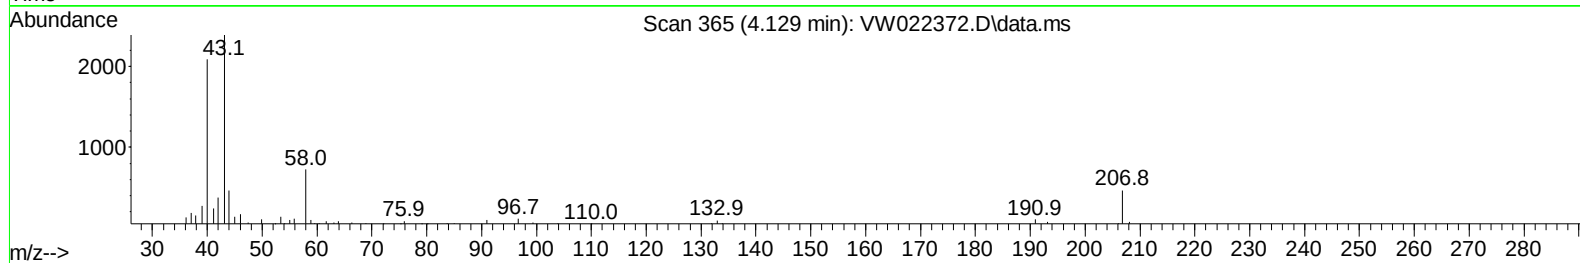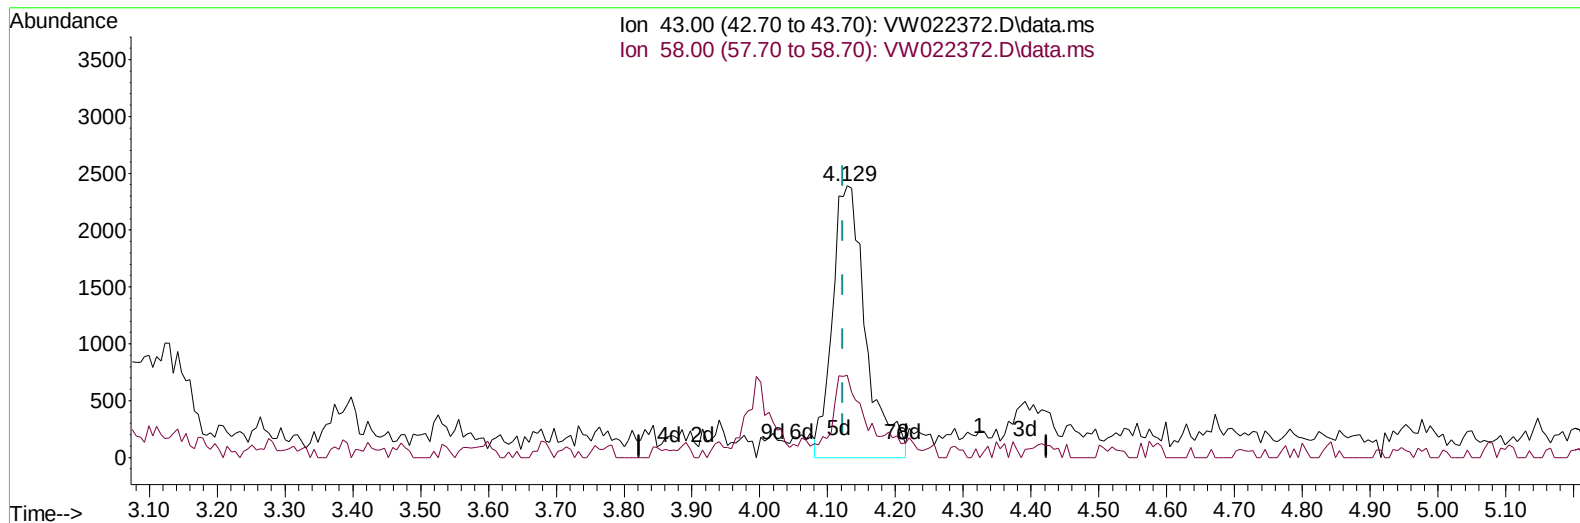

TIC: VW022372.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 13.41 ug/L m

response 8164

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	0.34
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022372.D
 Acq On : 01 Apr 2022 17:31
 Operator : SY/VA
 Sample : N2225-05
 Misc : 7.88g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQD4

Manual IntegrationsAPPROVED

Quant Time: Apr 02 02:36:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/02/2022
 Supervised By :Mahesh Dadoda 04/05/2022

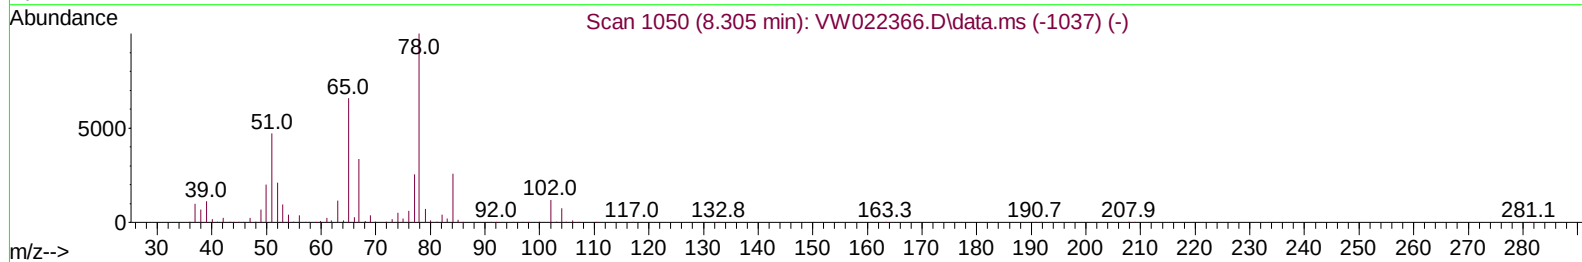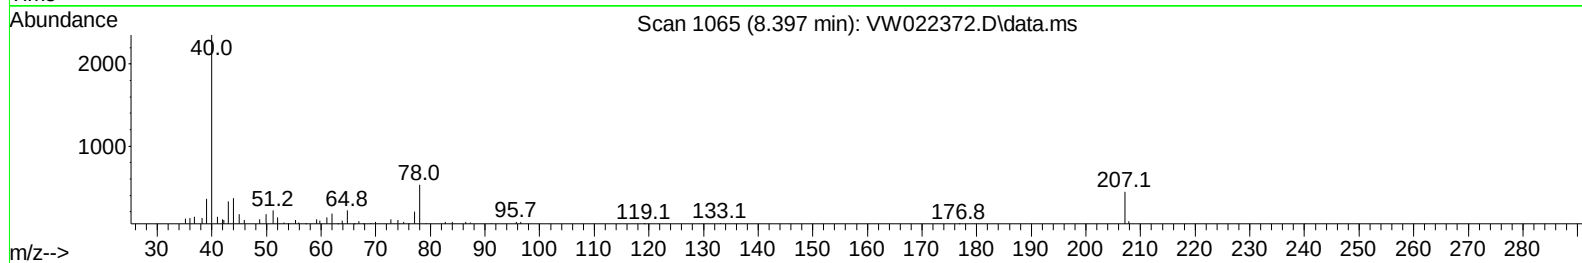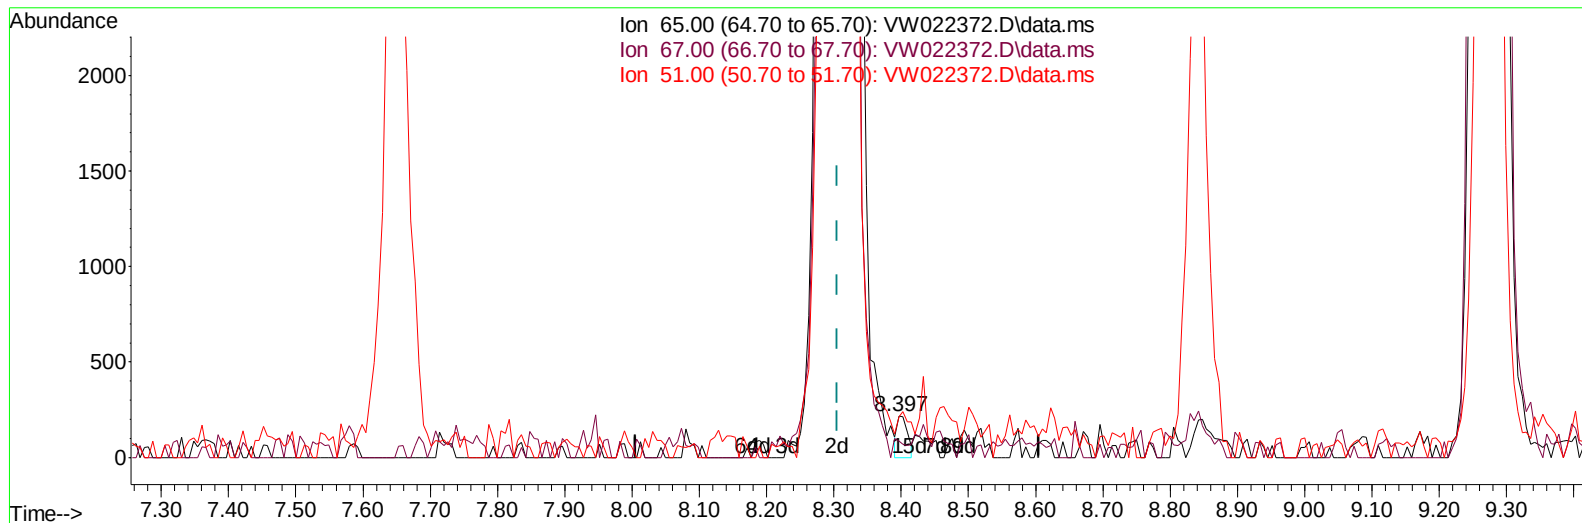

TIC: VW022372.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.397min (+ 0.092) 0.06 ug/L

response 229

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.50	50.66
51.00	90.00	86.90
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022372.D
 Acq On : 01 Apr 2022 17:31
 Operator : SY/VA
 Sample : N2225-05
 Misc : 7.88g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQD4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/02/2022
 Supervised By :Mahesh Dadoda 04/05/2022

Quant Time: Apr 02 02:36:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

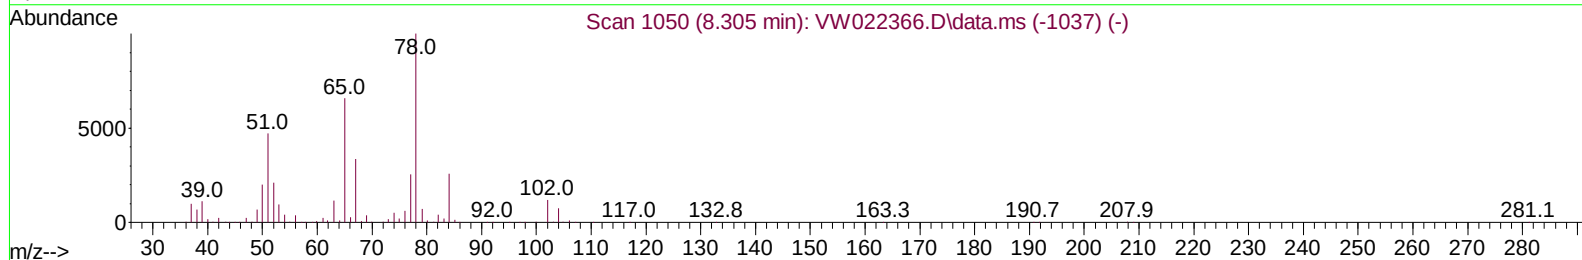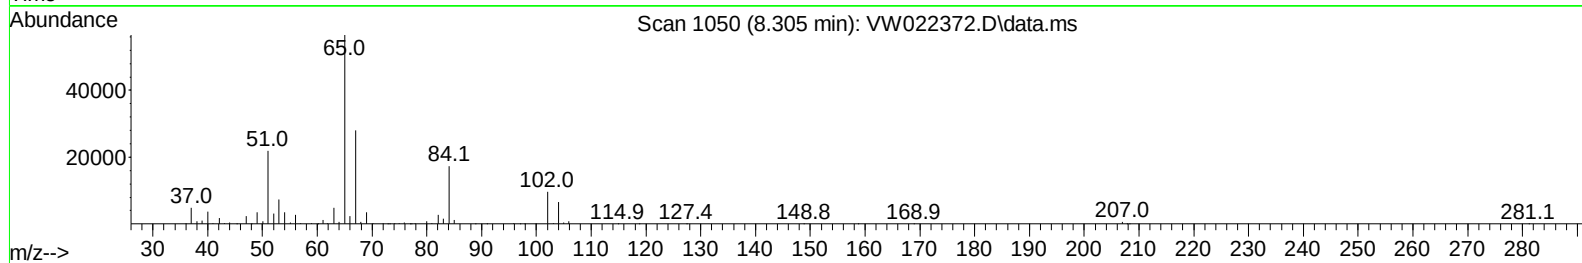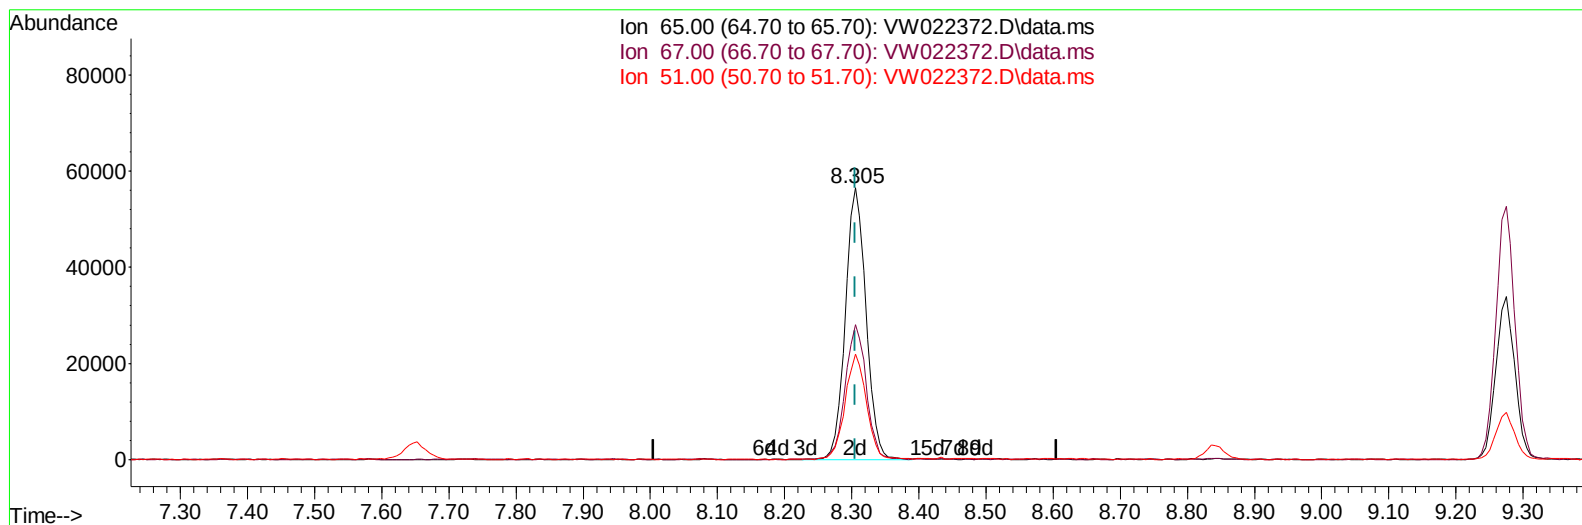

TIC: VW022372.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 32.96 ug/L m

response 120686

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.50	0.10#
51.00	90.00	0.16#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022372.D
 Acq On : 01 Apr 2022 17:31
 Operator : SY/VA
 Sample : N2225-05
 Misc : 7.88g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQD4

Manual IntegrationsAPPROVED

Quant Time: Apr 02 02:36:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/02/2022
 Supervised By :Mahesh Dadoda 04/05/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		222068	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117		219328	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		112915	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		106415	29.239	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	116.960%	
7) Chloroethane-d5	2.892	69		60865	28.013	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	112.040%	
11) 1,1-Dichloroethene-d2	4.026	63		101553	18.806	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	75.240%	
21) 2-Butanone-d5	7.074	46		87408	98.288	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	196.580%#	
24) Chloroform-d	7.653	84		164929	26.636	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	106.560%	
26) 1,2-Dichloroethane-d4	8.305	65		120686m	32.962	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	131.840%#	
32) Benzene-d6	8.275	84		336057	27.902	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	111.600%	
36) 1,2-Dichloropropane-d6	9.275	67		104680	28.950	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	115.800%	
41) Toluene-d8	10.323	98		326397	28.485	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	113.920%	
43) trans-1,3-Dichloroprop...	10.579	79		56400	31.018	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	124.080%	
47) 2-Hexanone-d5	10.921	63		70980	95.829	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	191.660%#	
56) 1,1,2,2-Tetrachloroeth...	12.689	84		115147	37.748	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	151.000%#	
66) 1,2-Dichlorobenzene-d4	13.853	152		104176	28.580	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	114.320%	
Target Compounds							
13) Acetone	4.129	43		8164m	13.406	ug/L	
42) Toluene	10.384	91		14785	0.944	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
Data File : VW022372.D
Acq On : 01 Apr 2022 17:31
Operator : SY/VA
Sample : N2225-05
Misc : 7.88g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGQD4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/02/2022
Supervised By :Mahesh Dadoda 04/05/2022

Quant Time: Apr 02 02:36:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 02 02:06:11 2022
Response via : Initial Calibration

