




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022374.D
 Acq On : 01 Apr 2022 18:19
 Operator : SY/VA
 Sample : N2225-07
 Misc : 7.18g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQD6

Manual IntegrationsAPPROVED

Quant Time: Apr 02 02:36:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/02/2022
 Supervised By :Mahesh Dadoda 04/06/2022

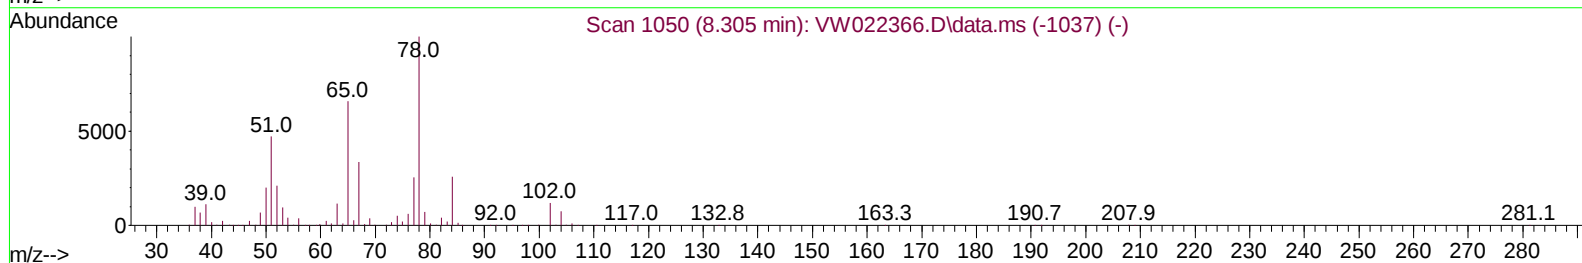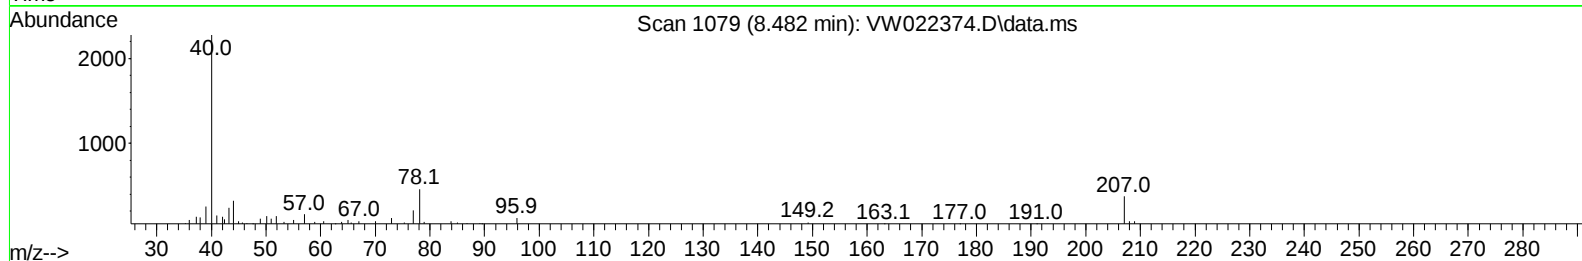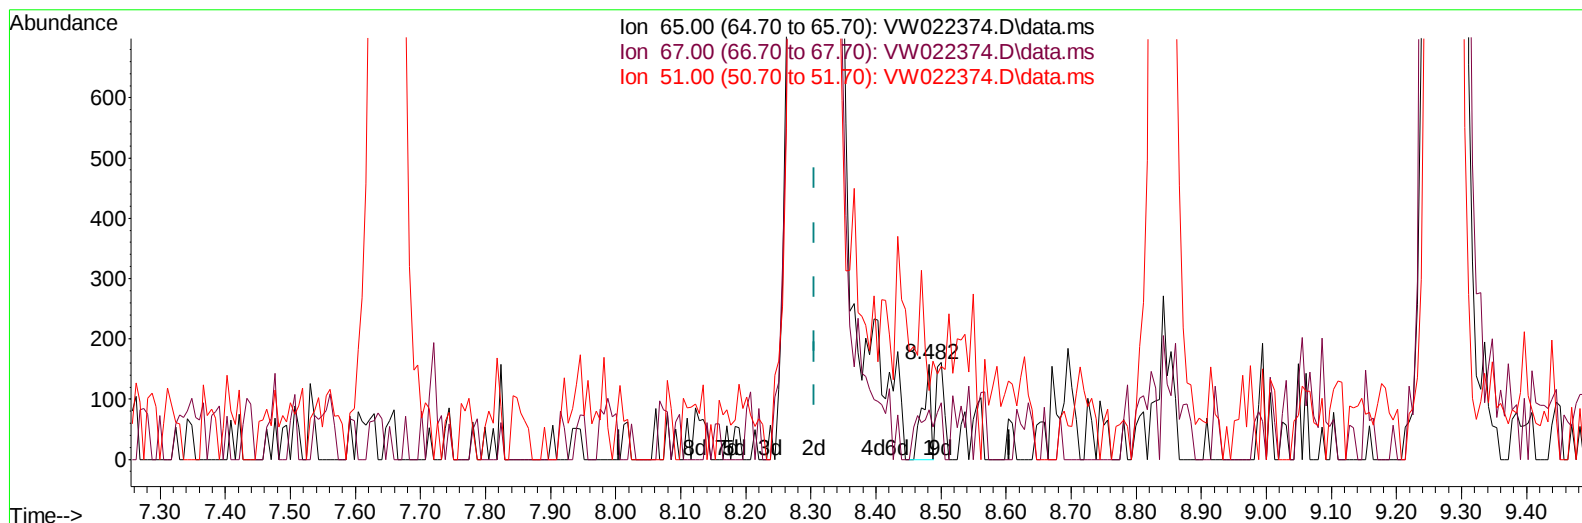

TIC: VW022374.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.482min (+ 0.177) 0.04 ug/L

response 140

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.50	52.14
51.00	90.00	80.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022374.D
 Acq On : 01 Apr 2022 18:19
 Operator : SY/VA
 Sample : N2225-07
 Misc : 7.18g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQD6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/02/2022
 Supervised By :Mahesh Dadoda 04/06/2022

Quant Time: Apr 02 02:36:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

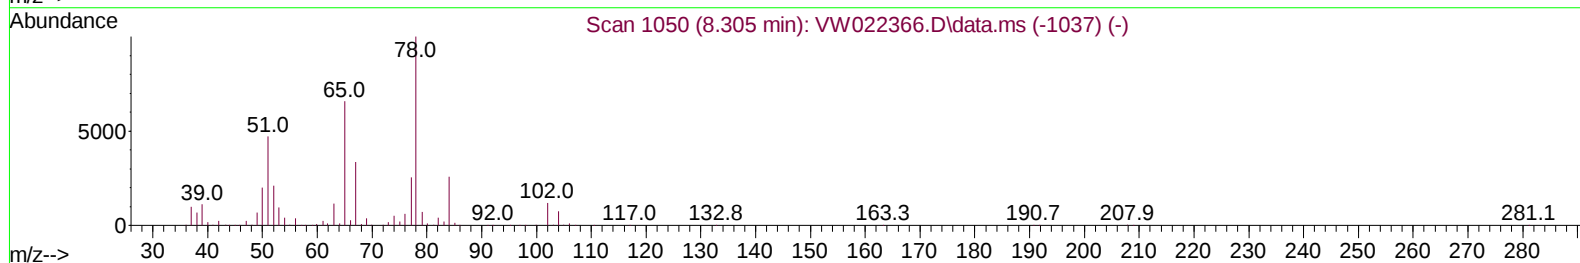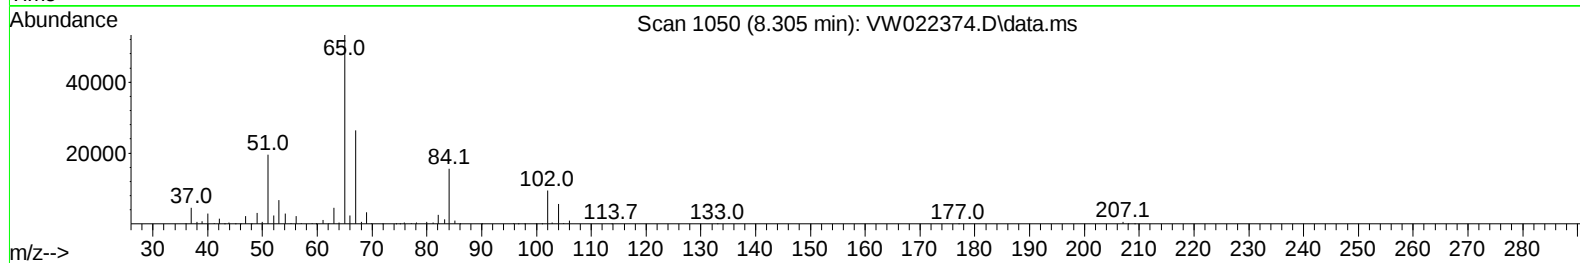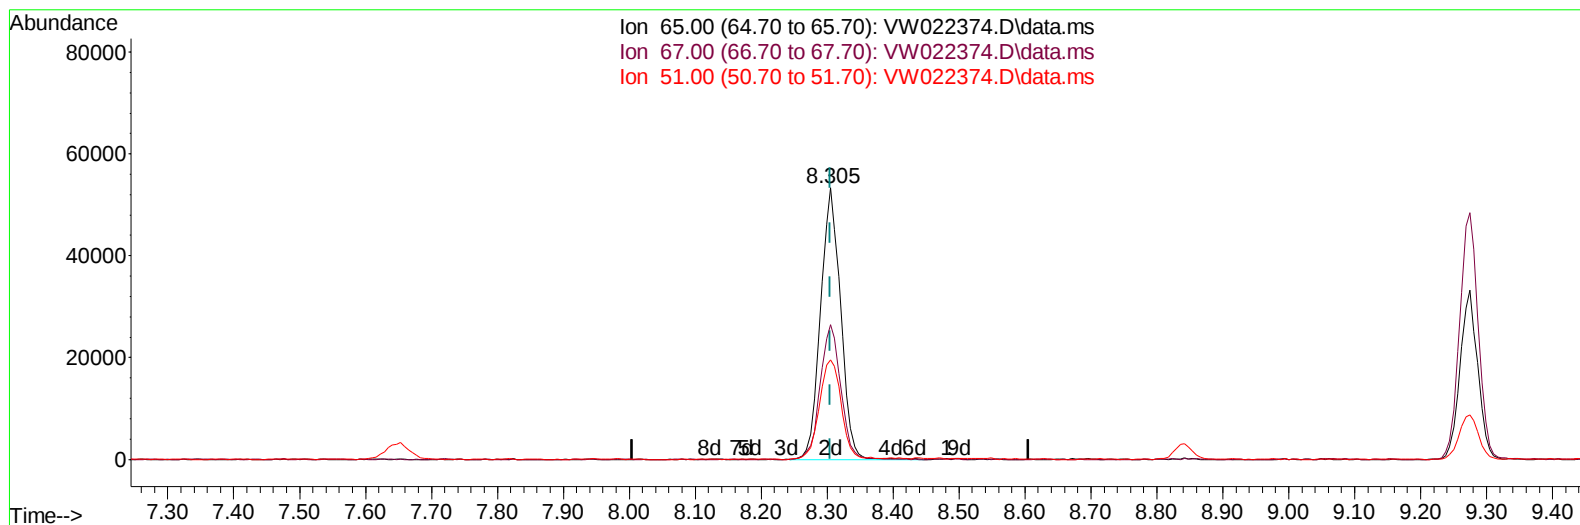

TIC: VW022374.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 33.27 ug/L m

response 112568

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.50	0.06#
51.00	90.00	0.10#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022374.D
 Acq On : 01 Apr 2022 18:19
 Operator : SY/VA
 Sample : N2225-07
 Misc : 7.18g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQD6

Manual IntegrationsAPPROVED

Quant Time: Apr 02 02:36:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/02/2022
 Supervised By :Mahesh Dadoda 04/06/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		205185	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117		198483	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		103868	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		102459	30.469	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	121.880%	
7) Chloroethane-d5	2.885	69		52896	26.349	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	105.400%	
11) 1,1-Dichloroethene-d2	4.019	63		92119	18.463	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110		Recovery	=	73.840%	
21) 2-Butanone-d5	7.074	46		76557	93.170	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	186.340%#	
24) Chloroform-d	7.647	84		151443	26.471	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	105.880%	
26) 1,2-Dichloroethane-d4	8.305	65		112568m	33.275	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	133.080%#	
32) Benzene-d6	8.275	84		314126	28.820	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	115.280%	
36) 1,2-Dichloropropane-d6	9.275	67		95012	29.036	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	116.160%	
41) Toluene-d8	10.323	98		302361	29.159	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	116.640%	
43) trans-1,3-Dichloroprop...	10.573	79		51672	31.402	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	125.600%	
47) 2-Hexanone-d5	10.921	63		62336	92.998	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	186.000%#	
56) 1,1,2,2-Tetrachloroeth...	12.689	84		104783	37.958	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	151.840%#	
66) 1,2-Dichlorobenzene-d4	13.847	152		96570	28.801	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	115.200%	
Target Compounds							
13) Acetone	4.129	43		3413	6.066	ug/L	60
42) Toluene	10.384	91		21981	1.551	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
Data File : VW022374.D
Acq On : 01 Apr 2022 18:19
Operator : SY/VA
Sample : N2225-07
Misc : 7.18g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGQD6

Manual IntegrationsAPPROVED

Quant Time: Apr 02 02:36:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 02 02:06:11 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/02/2022
Supervised By :Mahesh Dadoda 04/06/2022

