




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022376.D
 Acq On : 01 Apr 2022 19:07
 Operator : SY/VA
 Sample : N2179-02
 Misc : 6.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0R25

Manual IntegrationsAPPROVED

Quant Time: Apr 02 02:36:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/02/2022
 Supervised By :Mahesh Dadoda 04/05/2022

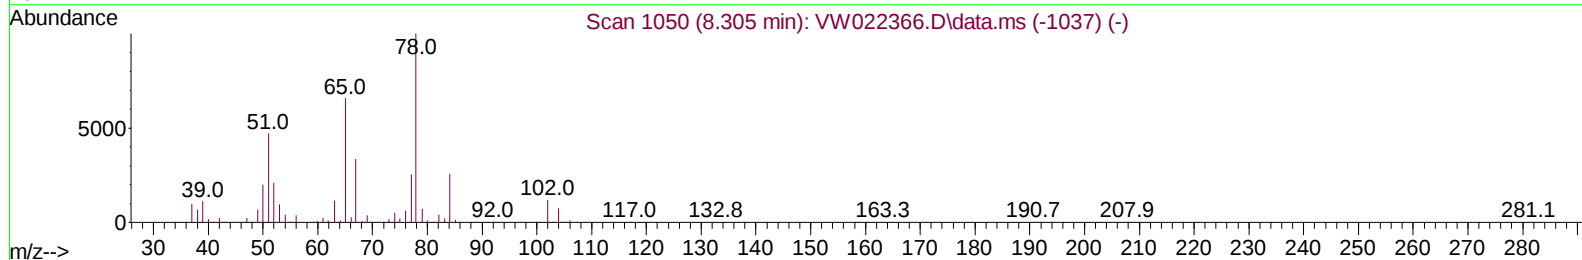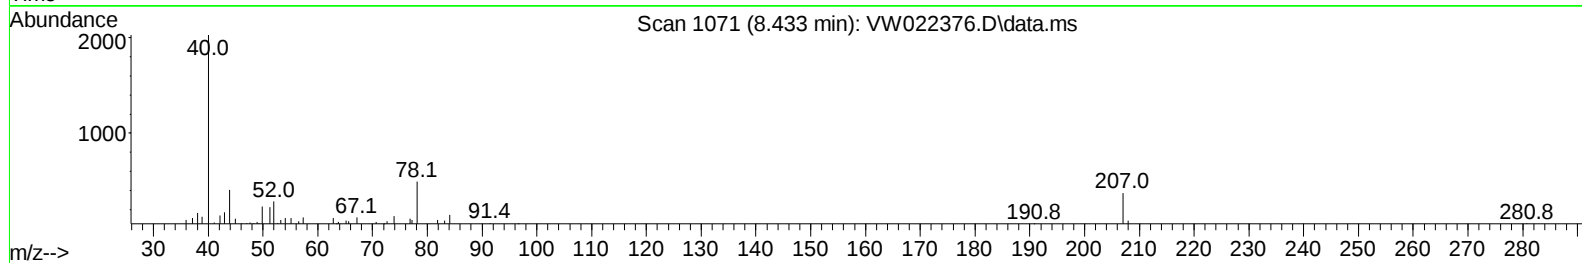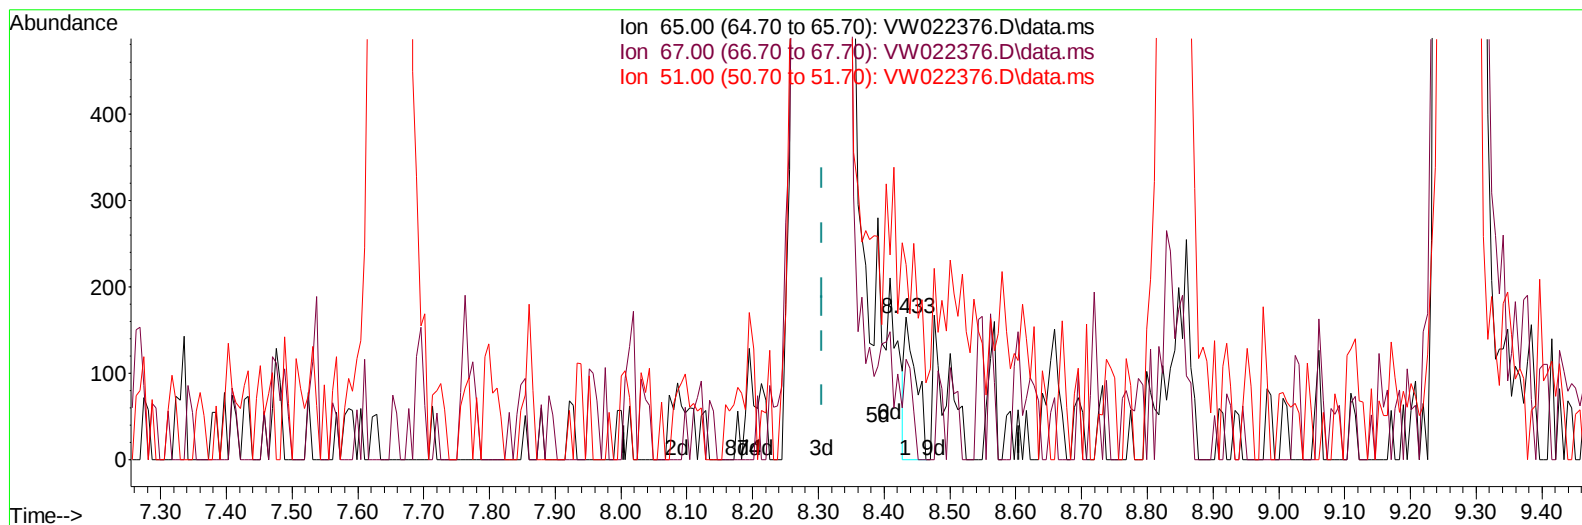

TIC: VW022376.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.433min (+ 0.128) 0.05 ug/L

response 207

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.50	49.28
51.00	90.00	69.57
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022376.D
 Acq On : 01 Apr 2022 19:07
 Operator : SY/VA
 Sample : N2179-02
 Misc : 6.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0R25

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/02/2022
 Supervised By :Mahesh Dadoda 04/05/2022

Quant Time: Apr 02 02:36:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

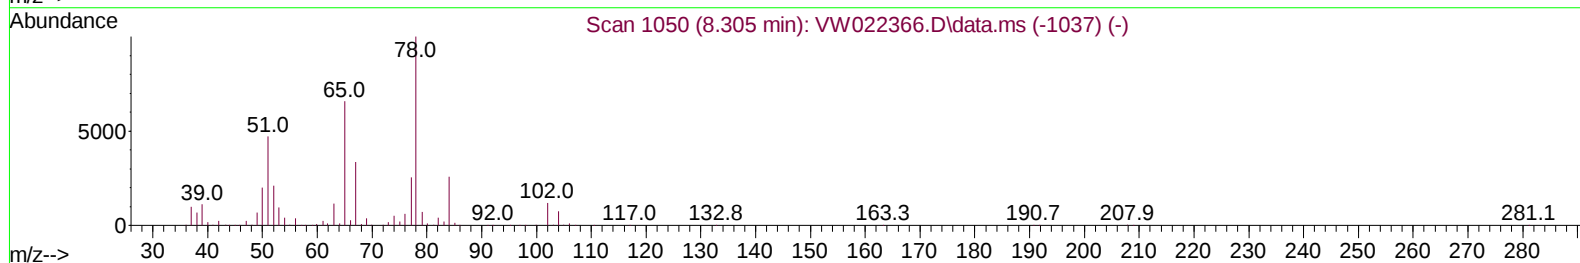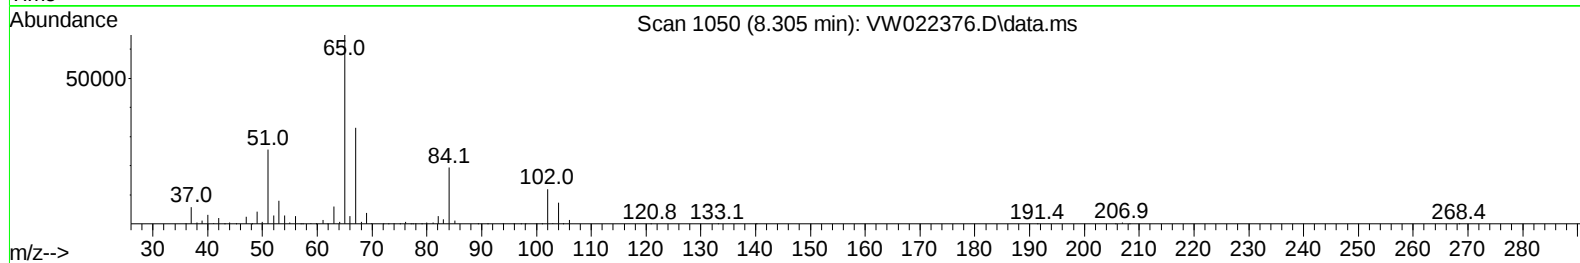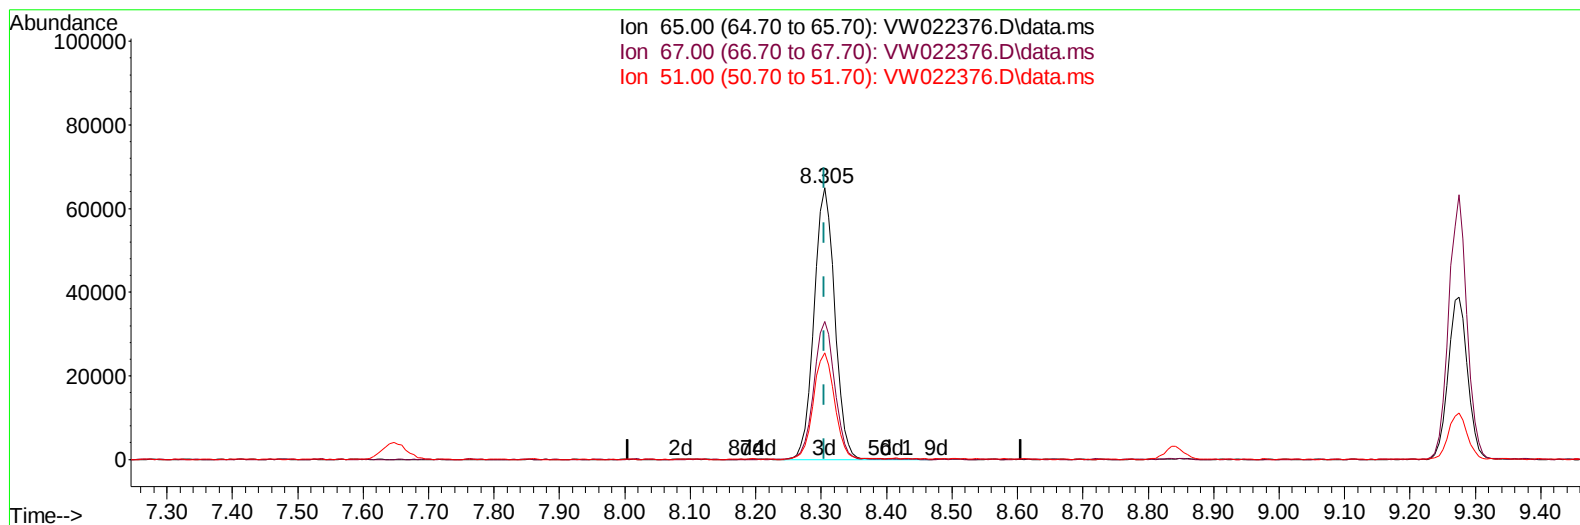

TIC: VW022376.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 34.98 ug/L m

response 143350

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.50	0.07#
51.00	90.00	0.10#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022376.D
 Acq On : 01 Apr 2022 19:07
 Operator : SY/VA
 Sample : N2179-02
 Misc : 6.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0R25

Manual IntegrationsAPPROVED

Quant Time: Apr 02 02:36:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/02/2022
 Supervised By :Mahesh Dadoda 04/05/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	248539	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	223331	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	98037	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	131579	32.303	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	129.200%	
7) Chloroethane-d5	2.885	69	71903	29.569	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	118.280%	
11) 1,1-Dichloroethene-d2	4.019	63	115197	19.061	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	76.240%	
21) 2-Butanone-d5	7.080	46	75986	76.344	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	152.680%#	
24) Chloroform-d	7.647	84	188722	27.233	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	108.920%	
26) 1,2-Dichloroethane-d4	8.305	65	143350m	34.983	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	139.920%#	
32) Benzene-d6	8.275	84	397919	32.446	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	129.800%	
36) 1,2-Dichloropropane-d6	9.275	67	123046	33.419	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	133.680%#	
41) Toluene-d8	10.323	98	375337	32.169	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	128.680%	
43) trans-1,3-Dichloroprop...	10.579	79	57098	30.839	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	123.360%	
47) 2-Hexanone-d5	10.921	63	62159	82.416	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	164.840%#	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	120004	38.635	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	154.560%#	
66) 1,2-Dichlorobenzene-d4	13.847	152	104317	32.961	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	131.840%#	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
Data File : VW022376.D
Acq On : 01 Apr 2022 19:07
Operator : SY/VA
Sample : N2179-02
Misc : 6.06g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0R25

Manual IntegrationsAPPROVED

Quant Time: Apr 02 02:36:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 02 02:06:11 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/02/2022
Supervised By :Mahesh Dadoda 04/05/2022

