




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022379.D
 Acq On : 01 Apr 2022 20:20
 Operator : SY/VA
 Sample : VIBLK409
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK409

Manual IntegrationsAPPROVED

Quant Time: Apr 02 02:37:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/02/2022
 Supervised By :Mahesh Dadoda 04/06/2022

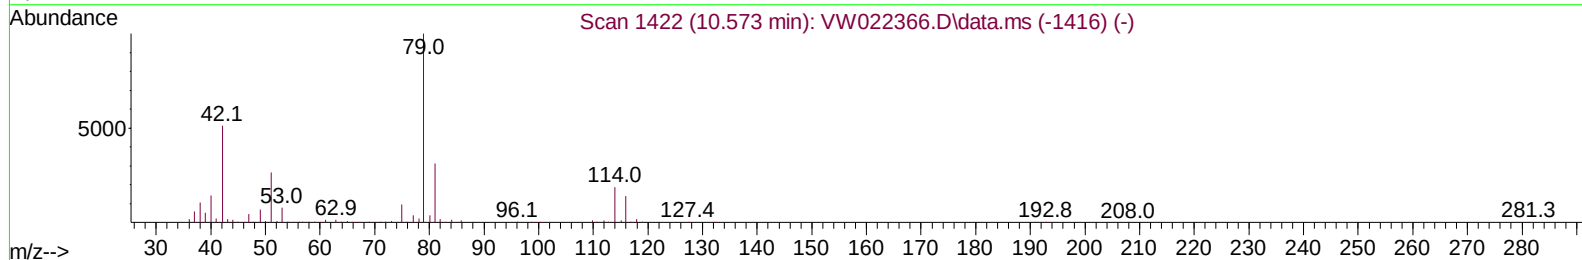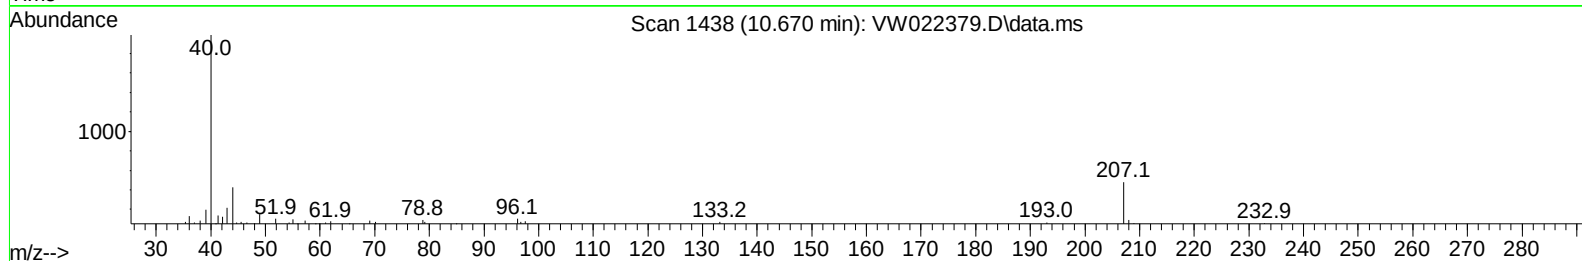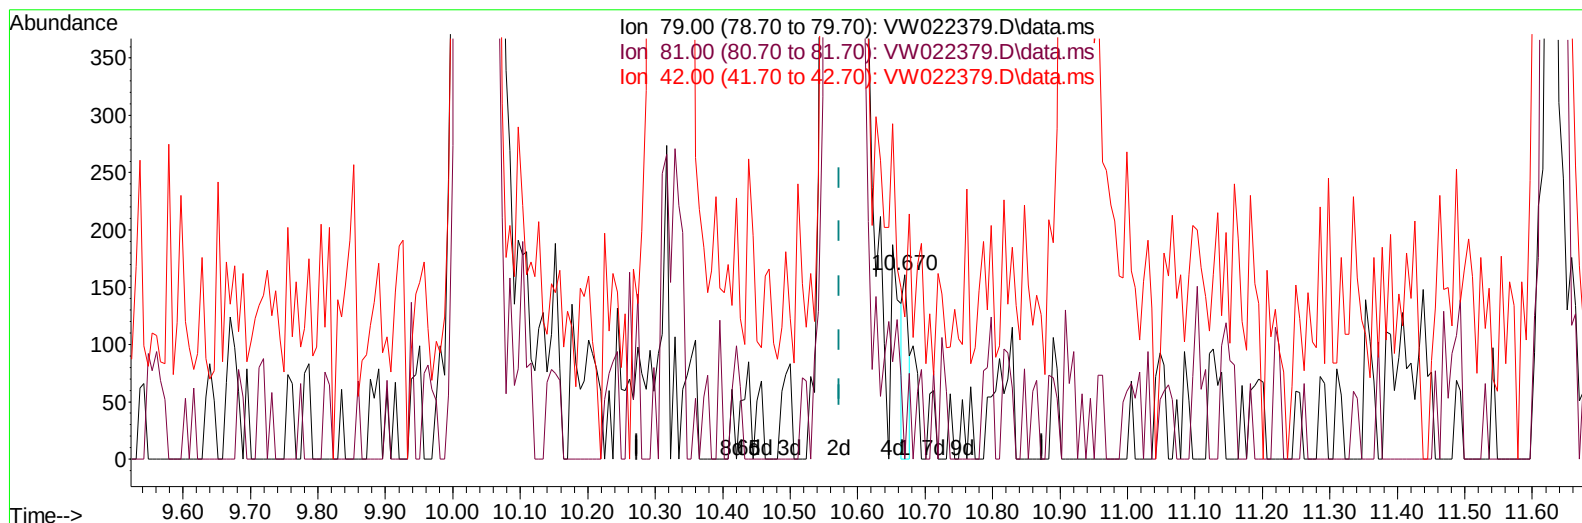

TIC: VW022379.D\data.ms

(43) trans-1,3-Dichloropropene-d4 (S)

10.670min (+ 0.097) 0.05 ug/L

response 92

Ion	Exp%	Act%
79.00	100.00	100.00
81.00	35.10	29.35
42.00	40.20	43.48
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022379.D
 Acq On : 01 Apr 2022 20:20
 Operator : SY/VA
 Sample : VIBLK409
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK409

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/02/2022
 Supervised By :Mahesh Dadoda 04/06/2022

Quant Time: Apr 02 02:37:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	237628	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	229758	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	107050	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	117311	30.122	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 120.480%			
7) Chloroethane-d5	2.891	69	70912	30.500	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 122.000%			
11) 1,1-Dichloroethene-d2	4.019	63	106657	18.458	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery = 73.840%			
21) 2-Butanone-d5	7.079	46	53841	56.579	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 113.160%			
24) Chloroform-d	7.652	84	175692	26.517	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 106.080%			
26) 1,2-Dichloroethane-d4	8.305	65	114321	29.179	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 116.720%			
32) Benzene-d6	8.274	84	378142	29.971	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 119.880%			
36) 1,2-Dichloropropane-d6	9.274	67	112428	29.681	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 118.720%			
41) Toluene-d8	10.323	98	368064	30.663	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 122.640%			
43) trans-1,3-Dichloroprop...	10.573	79	52819m	27.730	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 110.920%			
47) 2-Hexanone-d5	10.920	63	46004	59.290	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 118.580%			
56) 1,1,2,2-Tetrachloroeth...	12.694	84	88593	27.725	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 110.880%			
66) 1,2-Dichlorobenzene-d4	13.853	152	111197	32.177	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 128.720%#			

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
Data File : VW022379.D
Acq On : 01 Apr 2022 20:20
Operator : SY/VA
Sample : VIBLK409
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK409

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/02/2022
Supervised By :Mahesh Dadoda 04/06/2022

Quant Time: Apr 02 02:37:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 02 02:06:11 2022
Response via : Initial Calibration

