

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
 Data File : VW022373.D
 Acq On : 01 Apr 2022 17:55
 Operator : SY/VA
 Sample : N2225-06
 Misc : 7.48g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQD5

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/02/2022
 Supervised By : Mahesh Dadoda 04/05/2022

Quant Time: Apr 02 02:36:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 02 02:06:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	308815	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	294910	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	145960	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	127011	25.095	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.400%
7) Chloroethane-d5	2.885	69	73388	24.289	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.160%
11) 1,1-Dichloroethene-d2	4.019	63	120662	16.068	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.280%
21) 2-Butanone-d5	7.074	46	65285	52.790	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.580%
24) Chloroform-d	7.647	84	196351	22.803	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.200%
26) 1,2-Dichloroethane-d4	8.305	65	131009m	25.731	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.920%
32) Benzene-d6	8.275	84	408042	25.196	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.800%
36) 1,2-Dichloropropane-d6	9.274	67	122153	25.124	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.480%
41) Toluene-d8	10.323	98	385962m	25.051	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.200%
43) trans-1,3-Dichloroprop...	10.579	79	60179	24.614	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.440%
47) 2-Hexanone-d5	10.920	63	53969	54.189	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.380%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	103854	25.320	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.280%
66) 1,2-Dichlorobenzene-d4	13.853	152	118424	25.133	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.520%
Target Compounds					Qvalue	
42) Toluene	10.390	91	21475	1.020	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040122\
Data File : VW022373.D
Acq On : 01 Apr 2022 17:55
Operator : SY/VA
Sample : N2225-06
Misc : 7.48g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BGQD5

Quant Time: Apr 02 02:36:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 02 02:06:11 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 04/02/2022
Supervised By : Mahesh Dadoda 04/05/2022

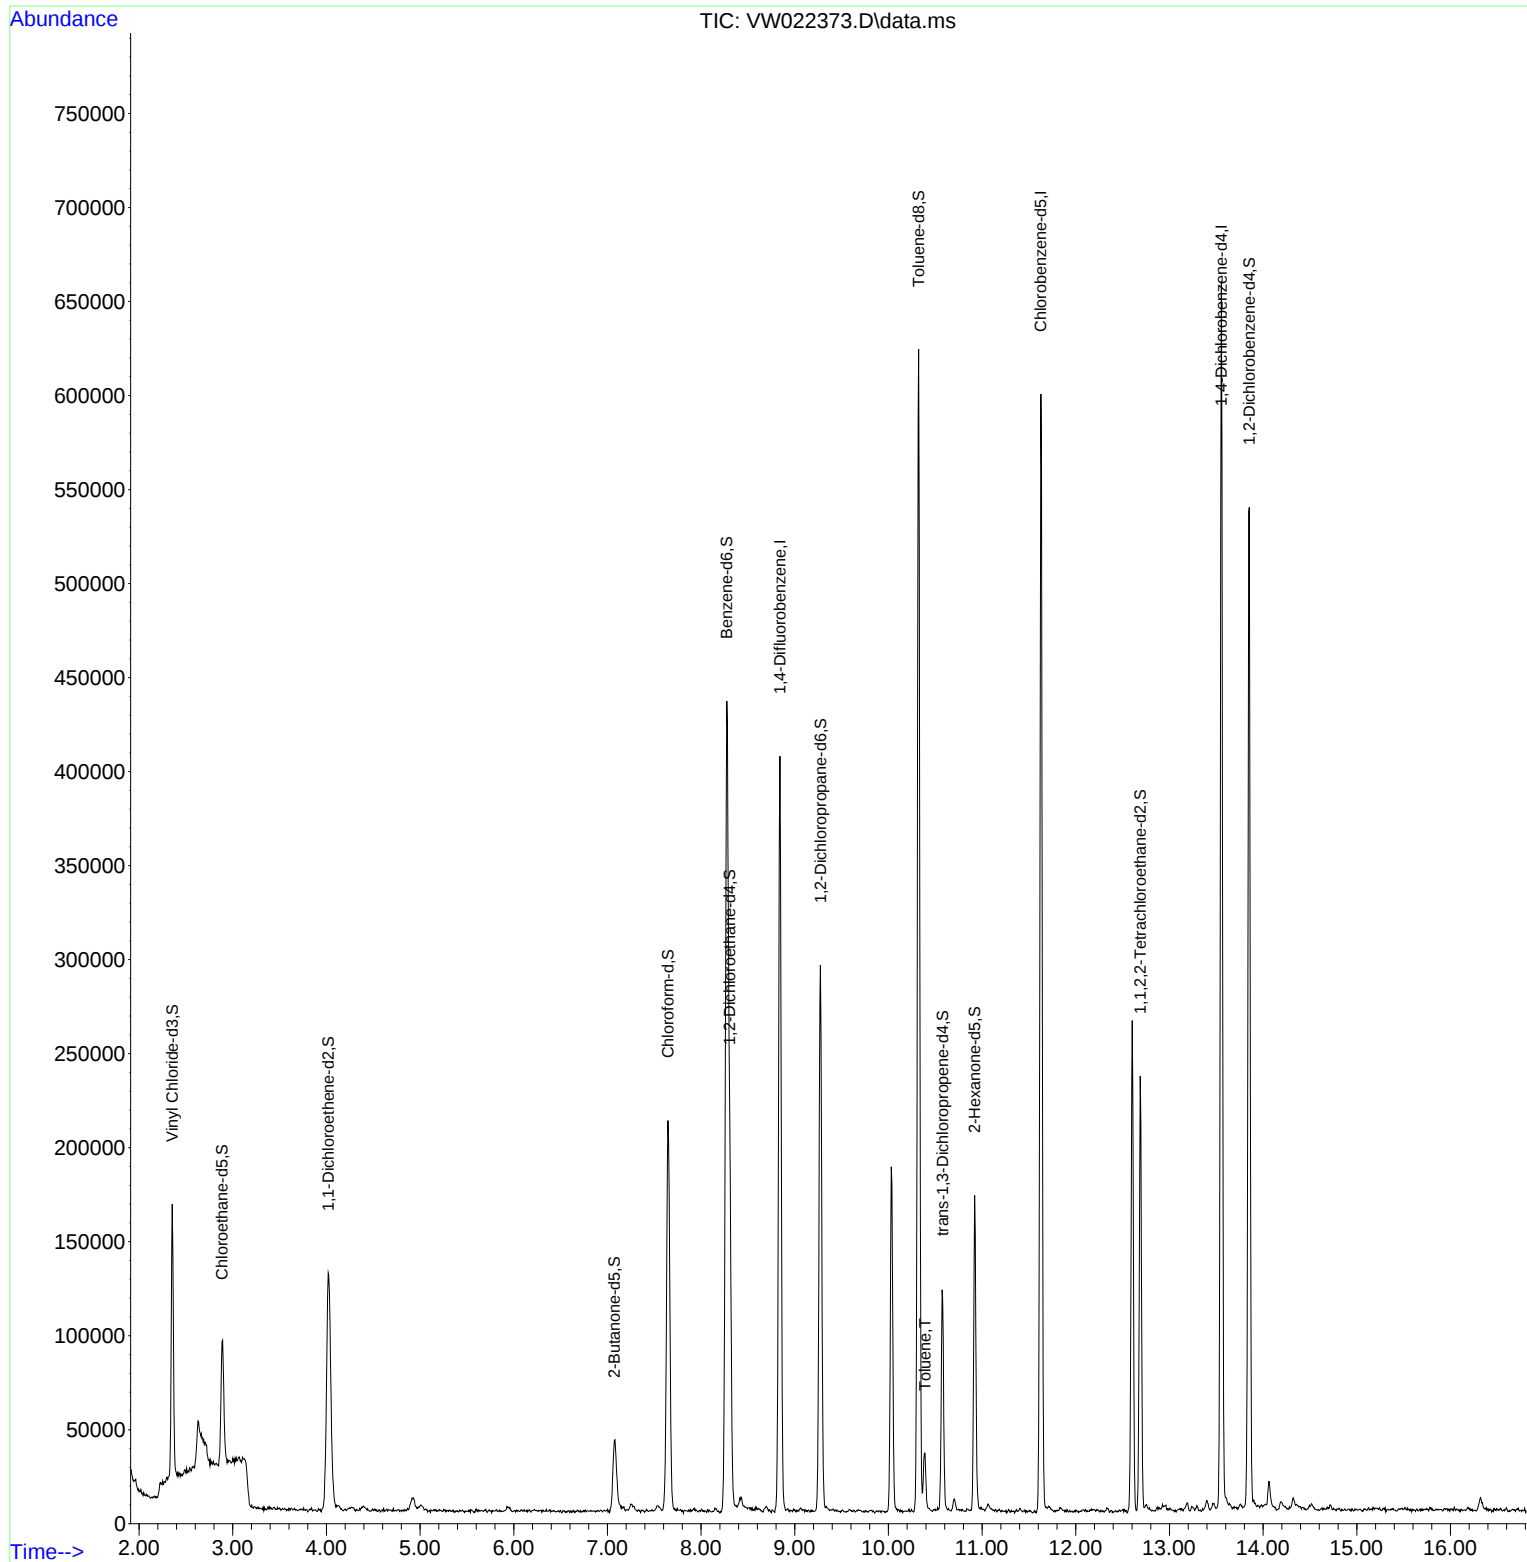

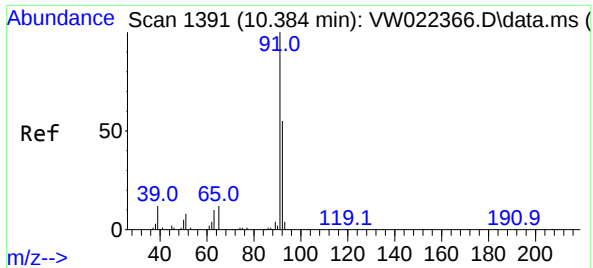

#42
Toluene
Concen: 1.020 ug/L
RT: 10.390 min Scan# 11
Delta R.T. 0.006 min
Lab File: VW022373.D
Acq: 01 Apr 2022 17:55

Instrument :
MSVOA_W
ClientSampleId :
BGQD5

Tgt Ion: 91 Resp: 21475
Ion Ratio Lower Upper
91 100
92 56.7 40.4 75.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/02/2022
Supervised By :Mahesh Dadoda 04/05/2022

