
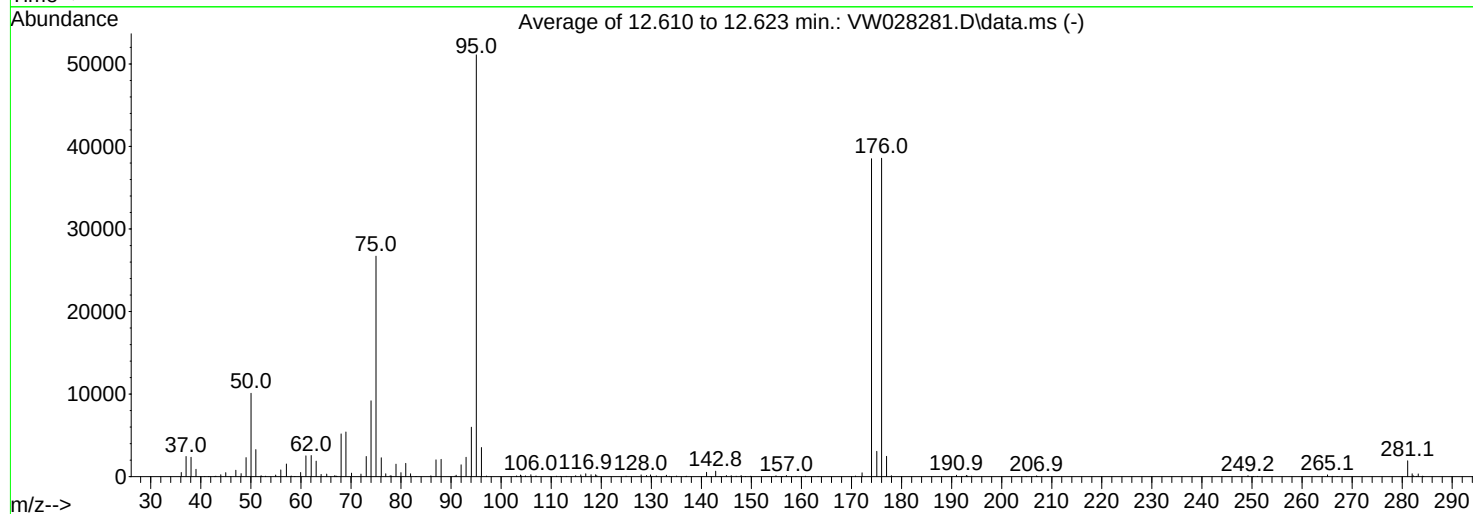


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040124\
Data File : VW028281.D
Acq On : 01 Apr 2024 13:30
Operator : SY/MD
Sample : BFB462
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB462

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Title : SFAM01.0
Last Update : Tue Apr 02 01:37:46 2024

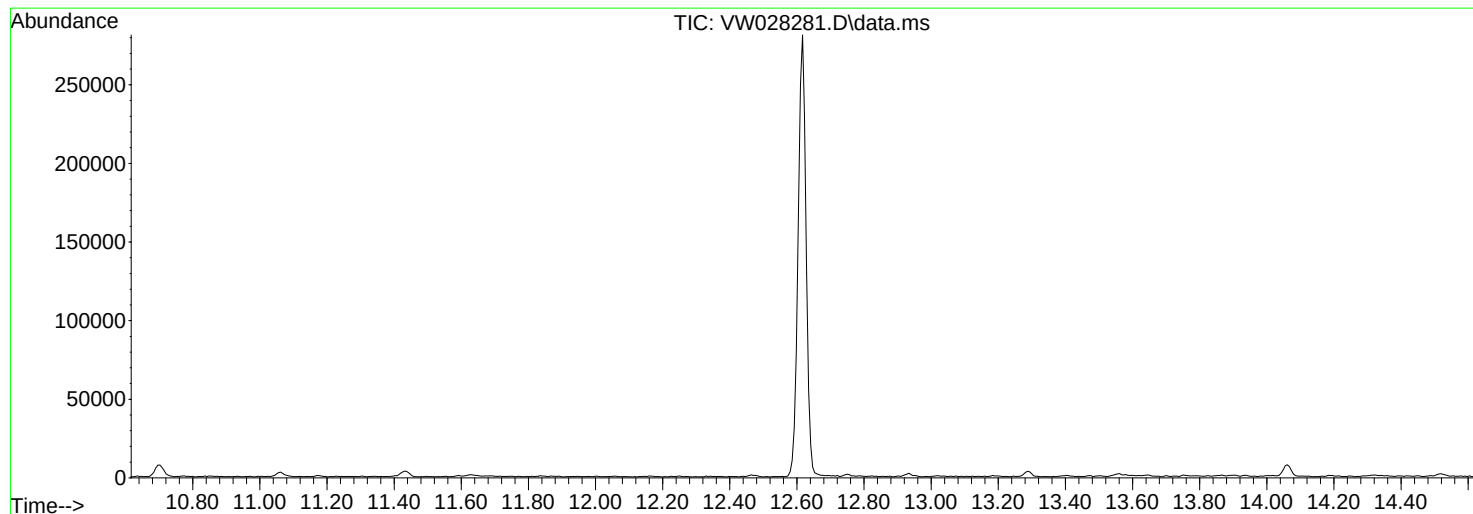

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	10105	PASS
75	95	30	80	52.3	26712	PASS
95	95	100	100	100.0	51099	PASS
96	95	5	9	6.9	3535	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.4	38517	PASS
175	174	5	9	8.0	3065	PASS
176	174	95	101	100.1	38571	PASS
177	176	5	9	6.4	2470	PASS

m/z	Abundance
39.90	587.0
44.00	188.0
52.20	51.0

Instrument :
MSVOA_W
ClientSampleId :
BFB462

m/z	Abundance
36.10	442.0
37.10	2596.0
38.00	2419.0
39.10	894.0
40.00	492.0
40.80	52.0
41.60	62.0
43.00	104.0
44.00	387.0
45.00	506.0
46.00	83.0
47.00	920.0
48.10	364.0
49.10	2585.0
50.10	10403.0
51.00	3236.0
52.30	195.0
53.00	63.0
55.00	157.0
56.00	795.0
57.10	1600.0
58.00	77.0
58.80	64.0
59.90	548.0
61.00	2321.0
62.10	2808.0
63.10	1871.0
64.10	331.0
65.10	268.0
66.80	251.0
68.10	5310.0
69.00	5477.0
70.10	401.0
72.10	334.0
73.00	2645.0
74.00	9565.0
75.00	28080.0
76.10	2384.0
77.00	301.0
77.80	208.0
79.00	1573.0
80.00	461.0
81.00	1647.0
81.90	384.0
83.00	57.0
86.00	86.0
87.00	1909.0
88.10	2233.0
90.80	208.0
92.00	1286.0
93.00	2514.0
94.00	5644.0
95.10	50592.0
96.10	3541.0
97.20	127.0
103.10	95.0
103.90	250.0
104.90	92.0
105.90	194.0
107.00	98.0
109.90	77.0
115.00	103.0
115.90	208.0
117.00	363.0
118.00	270.0
118.90	408.0
124.90	87.0
128.00	221.0
129.10	186.0
129.90	175.0
130.90	118.0
133.00	403.0
133.70	140.0
135.10	95.0
136.80	78.0
141.00	514.0
141.90	72.0
142.80	542.0
145.00	158.0
145.90	110.0
147.00	99.0
148.00	176.0
148.80	66.0
154.90	101.0
157.10	106.0
160.80	75.0
163.30	62.0
170.80	121.0
172.00	436.0
174.00	34008.0
175.10	2693.0
176.00	34208.0

Instrument :
MSVOA_W
ClientSampleId :
BFB462

177.00	2254.0
177.90	103.0
191.00	285.0
192.00	61.0
193.00	365.0
193.90	93.0
204.90	55.0
206.90	119.0
249.10	188.0
250.30	56.0
251.10	97.0
265.10	328.0
266.20	67.0
267.00	50.0
281.10	3231.0
282.00	839.0
283.20	703.0
284.10	158.0

Instrument :
MSVOA_W
ClientSampleId :
BFB462

m/z	Abundance
36.10	636.0
37.00	2689.0
38.10	2517.0
39.10	993.0
39.90	592.0
43.00	70.0
44.00	437.0
45.00	584.0
46.90	777.0
48.10	429.0
49.10	2459.0
50.00	11365.0
51.00	3705.0
52.00	177.0
52.90	56.0
54.90	254.0
56.00	880.0
57.10	1620.0
58.10	81.0
60.00	615.0
61.00	2904.0
62.10	2779.0
63.10	2228.0
64.00	316.0
65.00	222.0
65.20	222.0
67.00	237.0
68.10	5715.0
69.00	6343.0
70.10	558.0
71.90	306.0
73.10	2720.0
74.00	10180.0
75.00	28976.0
76.10	2671.0
76.90	403.0
78.10	222.0
79.00	1759.0
80.00	624.0
81.00	1780.0
81.90	302.0
86.00	103.0
87.00	2447.0
88.00	2248.0
91.00	293.0
92.00	1631.0
93.00	2317.0
94.00	7211.0
95.00	57720.0
96.10	3841.0
97.00	86.0
103.00	112.0
103.80	313.0
104.90	111.0
105.90	316.0
107.00	118.0
111.10	115.0
111.90	135.0
113.00	95.0
114.90	147.0
115.80	211.0
116.80	376.0
118.00	226.0
119.10	375.0
125.00	89.0
127.90	277.0
129.10	73.0
129.80	231.0
131.00	87.0
133.00	86.0
135.10	83.0
137.00	105.0
141.10	511.0
142.90	826.0
145.00	149.0
145.90	128.0
146.90	70.0
147.90	123.0
149.90	84.0
154.90	104.0
156.20	82.0
156.90	138.0
160.80	75.0
170.80	87.0
172.10	547.0
174.00	40000.0
175.00	3412.0
176.00	44808.0
177.00	2866.0
177.90	145.0
190.90	167.0
192.10	52.0

Instrument :
MSVOA_W
ClientSampleId :
BFB462

192.80	129.0
193.20	149.0
194.00	81.0
207.00	160.0
249.20	95.0
265.10	210.0
266.10	52.0
281.10	1720.0
282.20	381.0
283.20	278.0
284.30	63.0

Instrument :
MSVOA_W
ClientSampleId :
BFB462

m/z	Abundance
36.10	425.0
37.00	2026.0
38.00	2108.0
39.00	817.0
40.00	673.0
42.70	51.0
44.00	413.0
45.00	385.0
47.10	639.0
48.00	345.0
49.00	1906.0
50.10	8547.0
51.00	2910.0
52.10	177.0
53.00	83.0
54.90	203.0
56.00	795.0
57.10	1380.0
58.10	75.0
60.00	333.0
61.00	2319.0
62.00	2083.0
63.00	1553.0
64.00	186.0
65.20	246.0
66.70	103.0
67.20	101.0
68.00	4488.0
69.00	4405.0
70.10	295.0
72.00	275.0
73.00	1942.0
74.00	7844.0
75.00	23080.0
76.00	1804.0
77.00	329.0
77.90	165.0
79.00	1232.0
80.00	375.0
80.90	1414.0
81.90	350.0
85.80	97.0
87.00	1743.0
87.90	1801.0
91.00	208.0
92.00	1402.0
93.00	2201.0
94.10	5119.0
95.00	44984.0
96.00	3223.0
103.20	84.0
104.10	246.0
104.80	76.0
106.00	176.0
106.80	90.0
111.00	60.0
114.80	79.0
116.00	204.0
116.90	287.0
117.90	234.0
118.90	280.0
127.90	170.0
129.00	146.0
129.80	224.0
131.10	60.0
133.00	67.0
135.00	72.0
137.00	83.0
140.00	55.0
141.00	550.0
142.90	636.0
143.80	85.0
144.90	96.0
146.00	105.0
147.90	116.0
149.90	78.0
154.90	131.0
155.90	56.0
157.00	152.0
158.90	100.0
170.80	51.0
172.20	396.0
174.00	41544.0
175.10	3091.0
176.00	36696.0
177.00	2290.0
178.00	88.0
191.10	60.0
193.20	111.0
207.20	112.0
249.30	65.0
265.10	79.0

Instrument :
MSVOA_W
ClientSampleId :
BFB462

281.20	801.0
282.00	227.0
282.90	95.0

Instrument :
MSVOA_W
ClientSampleId :
BFB462