

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040324\
 Data File : VW028296.D
 Acq On : 03 Apr 2024 16:21
 Operator : SY/MD
 Sample : P1965-02
 Misc : 2.85g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E07D4

Quant Time: Apr 04 03:04:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 04 03:01:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	367924	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	316243	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	130553	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	65896	15.307	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	61.240%
7) Chloroethane-d5	2.905	69	51860	17.243	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.960%
11) 1,1-Dichloroethene-d2	4.027	65	41475	15.193	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.760%
21) 2-Butanone-d5	7.075	46	51997	40.953	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.900%
24) Chloroform-d	7.648	84	192100	17.706	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	70.840%
26) 1,2-Dichloroethane-d4	8.307	65	105365	17.623	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	70.480%
32) Benzene-d6	8.276	84	372308	19.283	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	77.120%
36) 1,2-Dichloropropane-d6	9.270	67	116184	20.910	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.640%
41) Toluene-d8	10.325	98	329963	18.528	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	74.120%
43) trans-1,3-Dichloroprop...	10.575	79	45270	17.939	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.760%
47) 2-Hexanone-d5	10.922	63	40919	44.553	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.100%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	89470	21.798	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.200%
66) 1,2-Dichlorobenzene-d4	13.848	152	91221	19.181	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	76.720%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3292	0.413	ug/L	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040324\
Data File : VW028296.D
Acq On : 03 Apr 2024 16:21
Operator : SY/MD
Sample : P1965-02
Misc : 2.85g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E07D4

Quant Time: Apr 04 03:04:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 04 03:01:50 2024
Response via : Initial Calibration

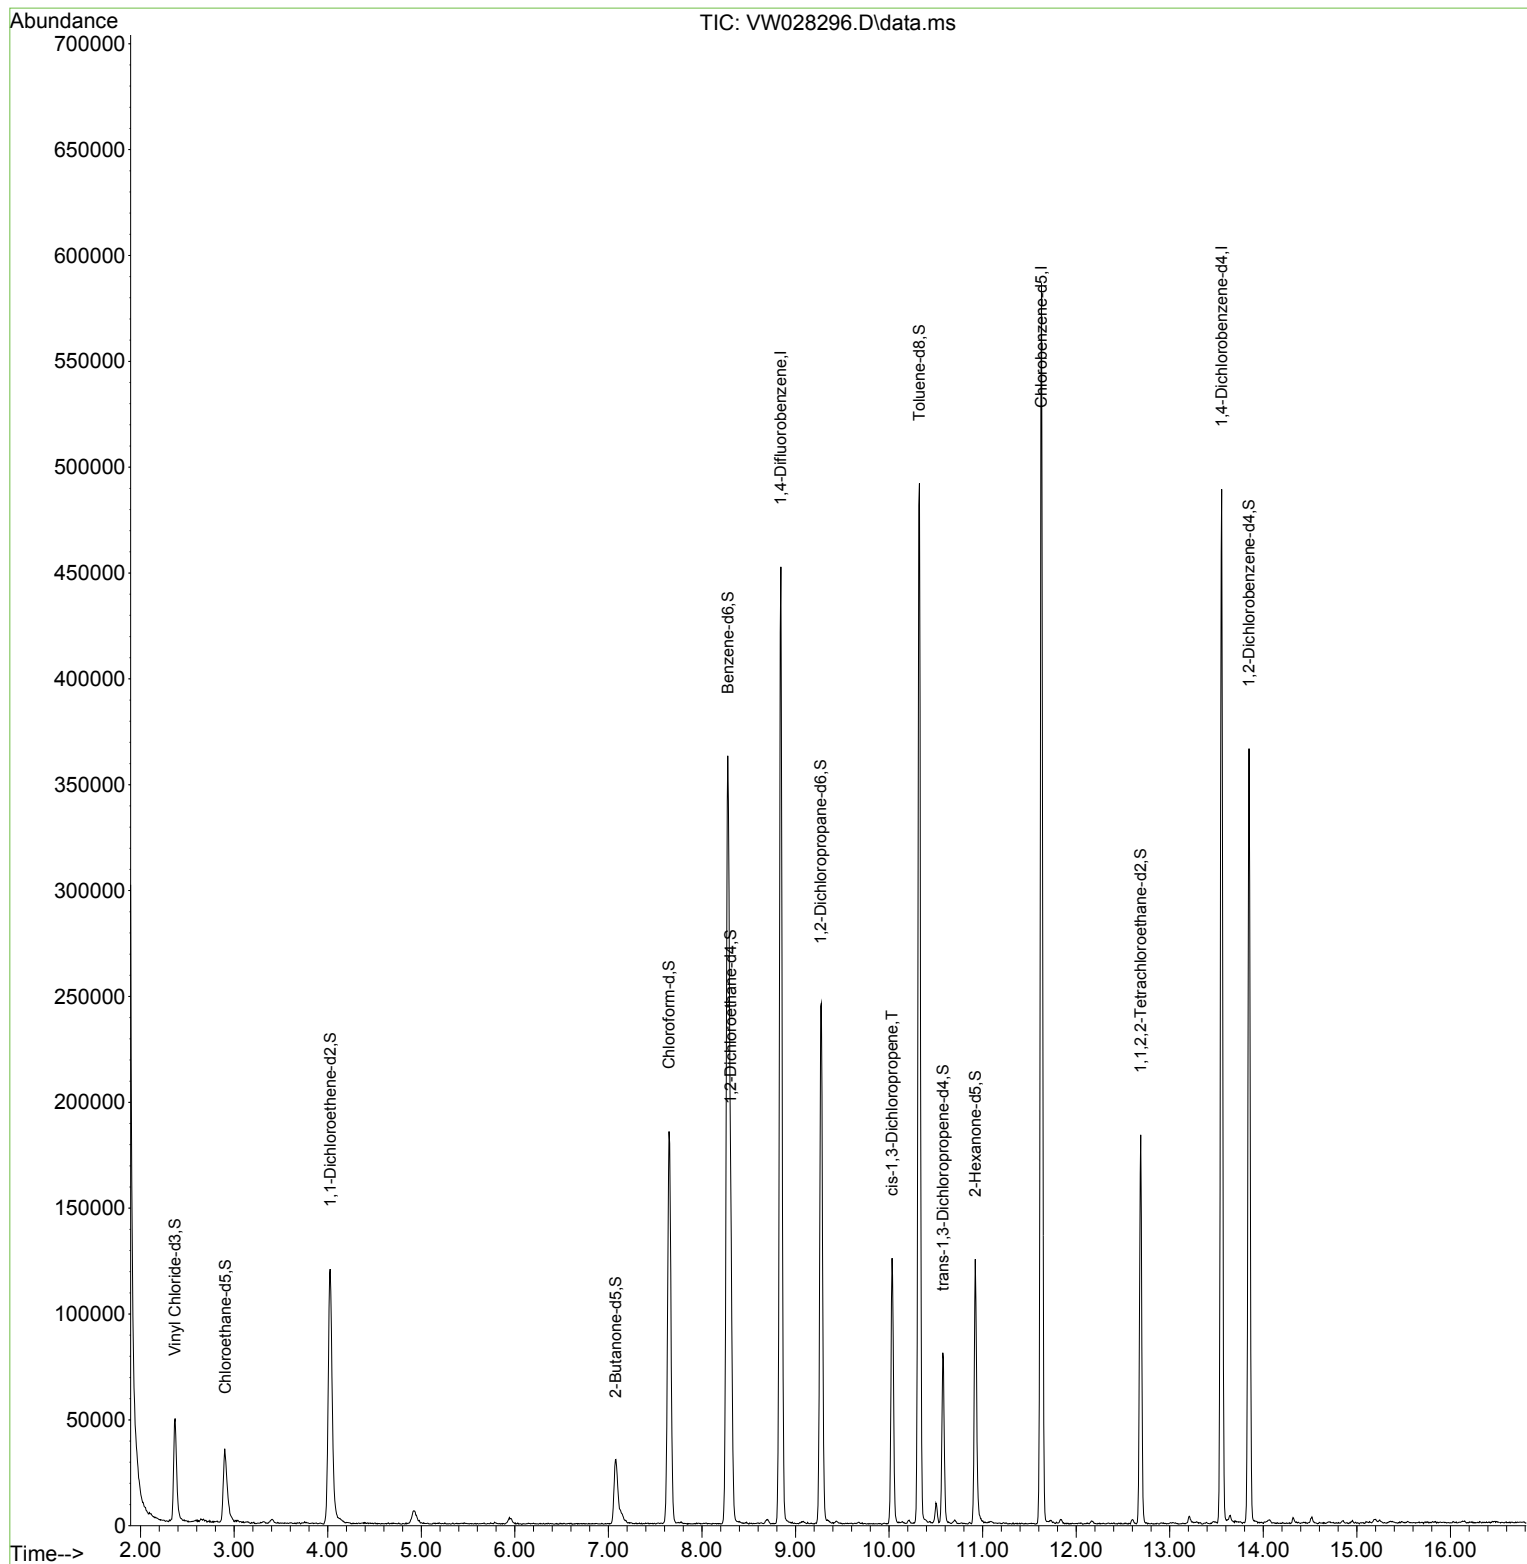

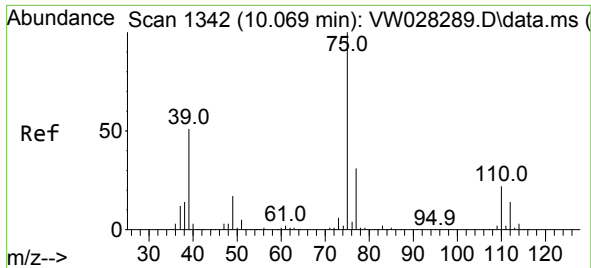

#39
 cis-1,3-Dichloropropene
 Concen: 0.413 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW028296.D
 Acq: 03 Apr 2024 16:21

Instrument :
 MSVOA_W
 ClientSampleId :
 E07D4

Tgt Ion: 75 Resp: 3292
 Ion Ratio Lower Upper
 75 100
 77 49.4 22.5 41.7#

