

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040324\
 Data File : VW028297.D
 Acq On : 03 Apr 2024 16:45
 Operator : SY/MD
 Sample : P1965-03
 Misc : 2.87g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E07D5

Quant Time: Apr 04 03:05:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 04 03:01:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	408158	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	346853	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	137190	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	72314	15.142	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.560%
7) Chloroethane-d5	2.899	69	58126	17.421	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.680%
11) 1,1-Dichloroethene-d2	4.027	65	47220	15.592	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.360%
21) 2-Butanone-d5	7.075	46	50463	35.827	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.660%
24) Chloroform-d	7.654	84	214119	17.791	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	71.160%
26) 1,2-Dichloroethane-d4	8.307	65	113627	17.132	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	68.520%#
32) Benzene-d6	8.276	84	418715	19.772	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.080%
36) 1,2-Dichloropropane-d6	9.270	67	127192	20.871	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.480%
41) Toluene-d8	10.319	98	368352	18.858	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	75.440%
43) trans-1,3-Dichloroprop...	10.575	79	46935	16.957	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	67.840%
47) 2-Hexanone-d5	10.922	63	39542	39.254	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.500%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	90636	20.134	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	80.520%
66) 1,2-Dichlorobenzene-d4	13.848	152	103602	20.730	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	82.920%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	3788	0.433	ug/L #	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040324\
Data File : VW028297.D
Acq On : 03 Apr 2024 16:45
Operator : SY/MD
Sample : P1965-03
Misc : 2.87g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E07D5

Quant Time: Apr 04 03:05:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 04 03:01:50 2024
Response via : Initial Calibration

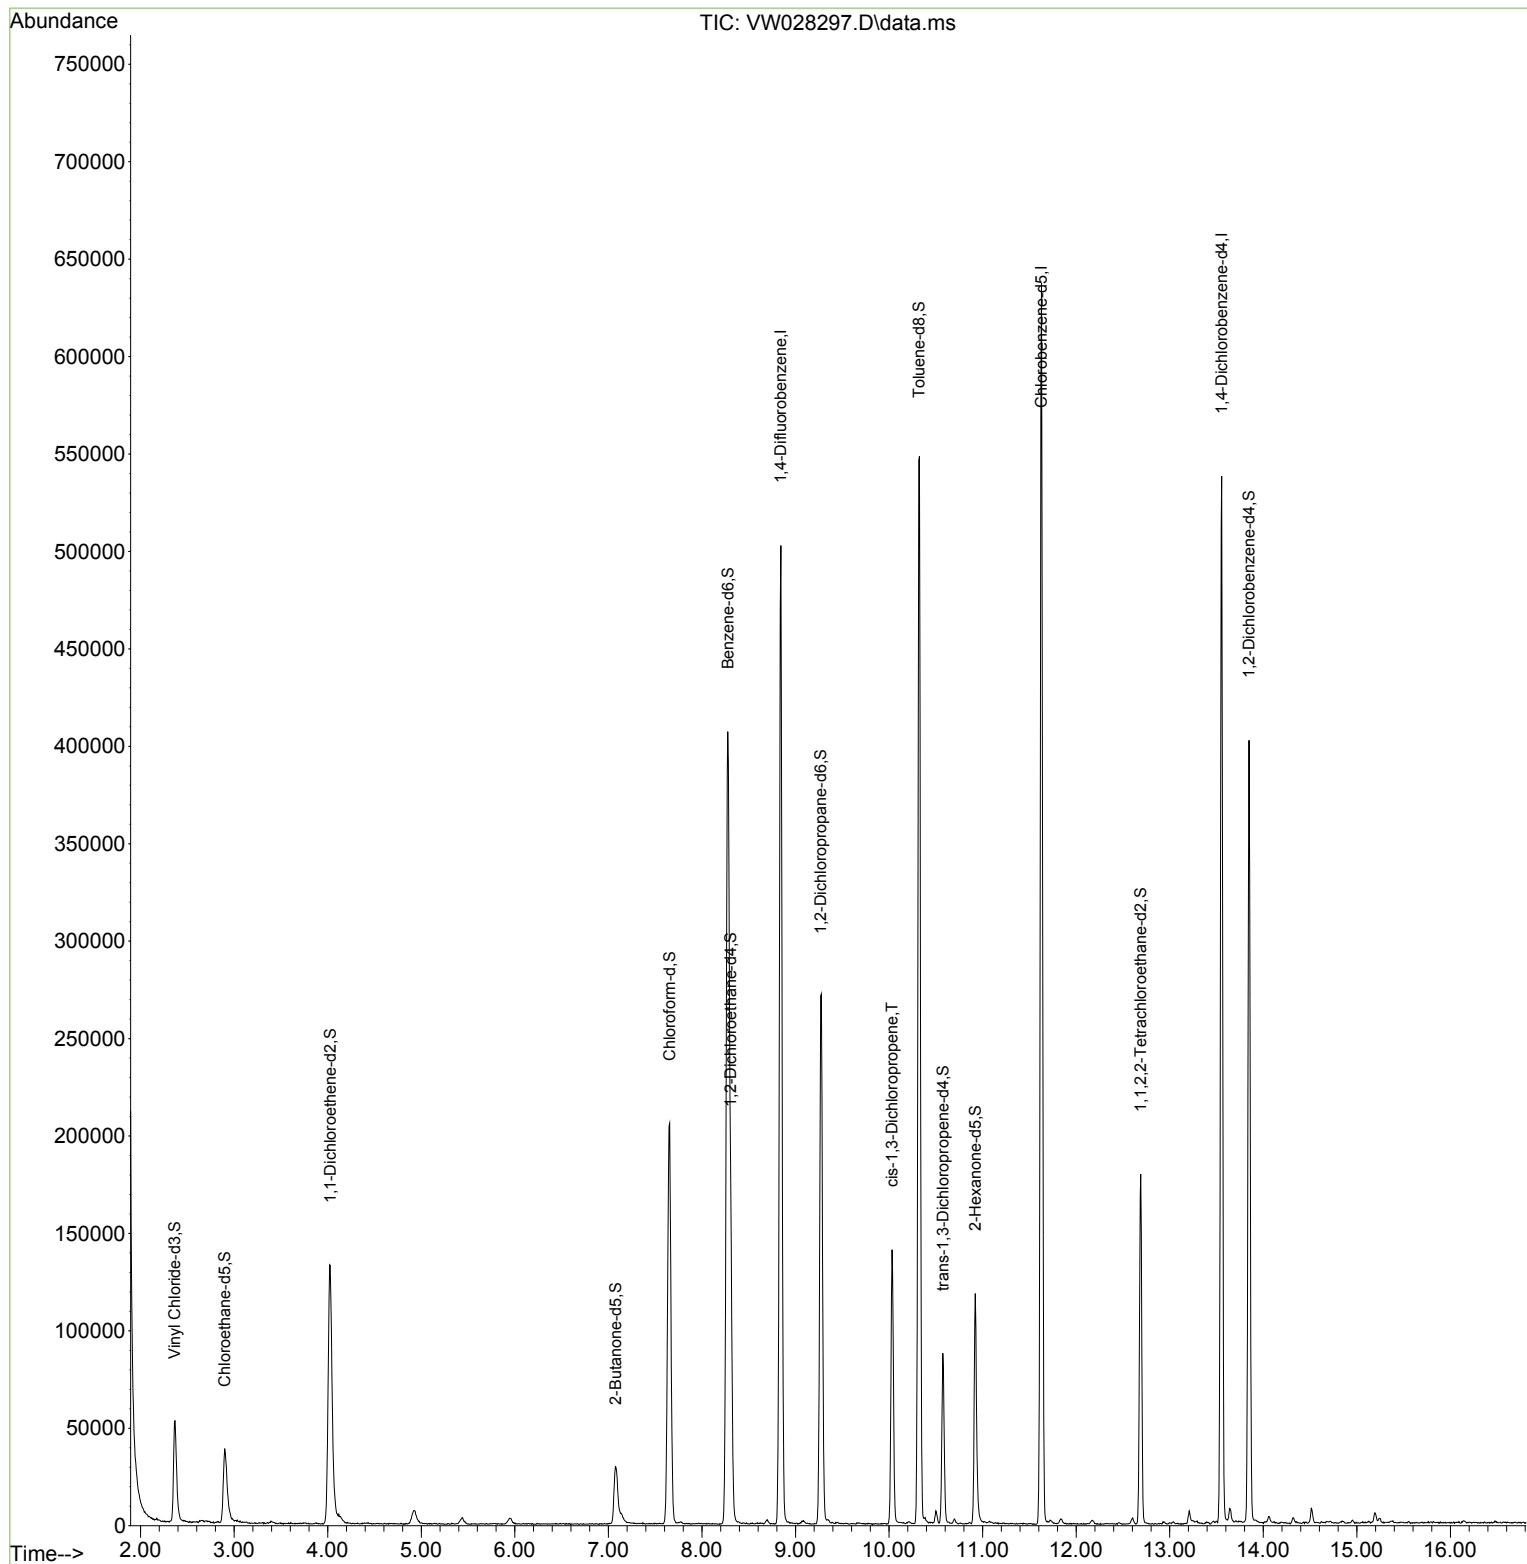

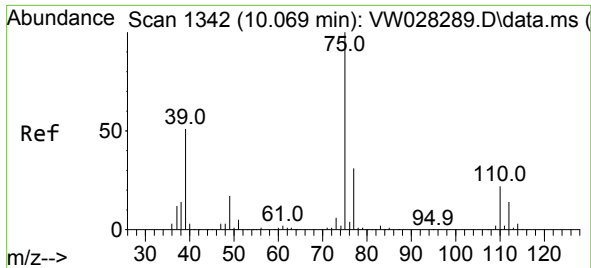

#39
 cis-1,3-Dichloropropene
 Concen: 0.433 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW028297.D
 Acq: 03 Apr 2024 16:45

Instrument :
 MSVOA_W
 ClientSampleId :
 E07D5

Tgt Ion: 75 Resp: 3788
 Ion Ratio Lower Upper
 75 100
 77 47.2 22.5 41.7#

