

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040324\
 Data File : VW028300.D
 Acq On : 03 Apr 2024 17:56
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK423

Quant Time: Apr 04 03:05:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 04 03:01:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	217038	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	205945	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	104625	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	41543	16.359	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.440%
7) Chloroethane-d5	2.905	69	36028	20.307	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.240%
11) 1,1-Dichloroethene-d2	4.027	65	27136	16.851	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.400%
21) 2-Butanone-d5	7.075	46	50225	67.057	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	134.120%
24) Chloroform-d	7.648	84	147363	23.026	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.120%
26) 1,2-Dichloroethane-d4	8.307	65	84080	23.840	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.360%
32) Benzene-d6	8.276	84	280139	22.280	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.120%
36) 1,2-Dichloropropane-d6	9.276	67	90877	25.115	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.480%
41) Toluene-d8	10.319	98	245101	21.134	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.520%
43) trans-1,3-Dichloroprop...	10.575	79	35452	21.572	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.280%
47) 2-Hexanone-d5	10.922	63	37906	63.376	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	126.760%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	79216	29.637	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	118.560%
66) 1,2-Dichlorobenzene-d4	13.848	152	94340	24.753	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.000%
Target Compounds						Qvalue
34) Trichloroethene	8.843	95	6876	1.945	ug/L	# 5


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040324\
Data File : VW028300.D
Acq On : 03 Apr 2024 17:56
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK423


Quant Time: Apr 04 03:05:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 04 03:01:50 2024
Response via : Initial Calibration

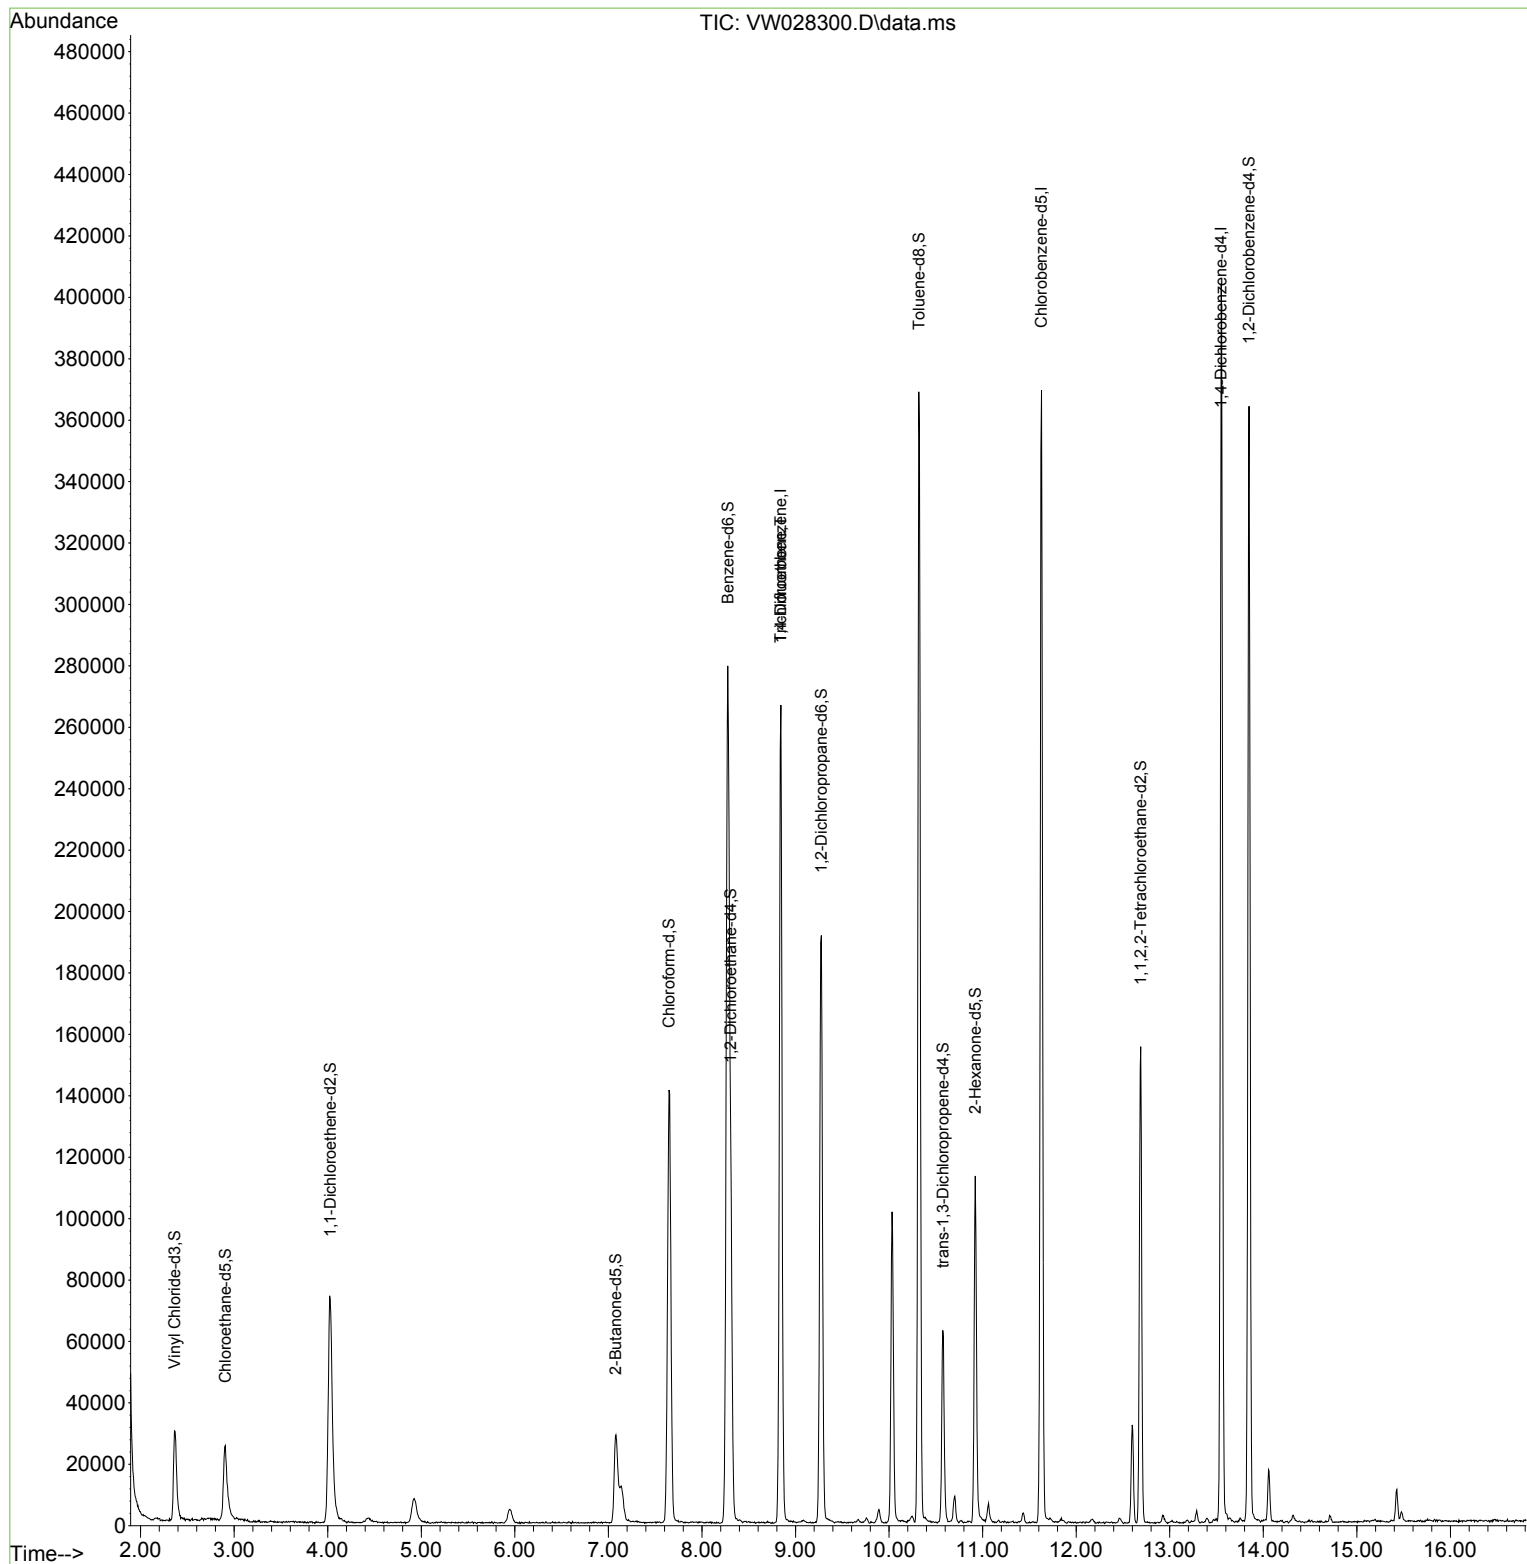

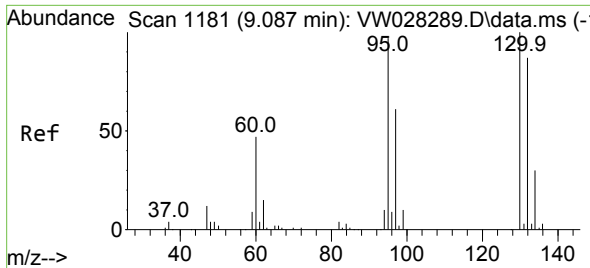

#34
 Trichloroethene
 Concen: 1.945 ug/L
 RT: 8.843 min Scan# 11
 Delta R.T. -0.244 min
 Lab File: VW028300.D
 Acq: 03 Apr 2024 17:56

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK423

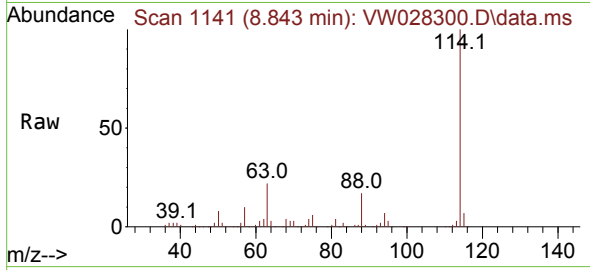

Tgt Ion: 95 Resp: 6876

Ion	Ratio	Lower	Upper
95	100		
97	0.0	42.4	78.6#
132	0.0	69.4	128.8#
130	0.0	69.7	129.4#

