

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040422\
 Data File : VW022391.D
 Acq On : 04 Apr 2022 17:05
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK410

Quant Time: Apr 05 01:57:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 05 01:44:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	212213	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	212330	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	110070	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	81393	23.402	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.600%
7) Chloroethane-d5	2.891	69	55798	26.874	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	107.480%
11) 1,1-Dichloroethene-d2	4.019	63	78313	15.176	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.720%
21) 2-Butanone-d5	7.080	46	33063	38.905	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.820%
24) Chloroform-d	7.653	84	118262	19.986	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.960%
26) 1,2-Dichloroethane-d4	8.305	65	73727	21.072	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	84.280%
32) Benzene-d6	8.275	84	250939	21.522	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.080%
36) 1,2-Dichloropropane-d6	9.274	67	70890	20.251	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	81.000%
41) Toluene-d8	10.427	98	121	0.011	ug/L	0.10
Spiked Amount	25.000	Range	30 - 130	Recovery	=	0.040%#
43) trans-1,3-Dichloroprop...	10.640	79	255	0.145	ug/L	0.06
Spiked Amount	25.000	Range	30 - 135	Recovery	=	0.560%#
47) 2-Hexanone-d5	10.920	63	28005	39.055	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.120%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	59832	20.261	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.040%
66) 1,2-Dichlorobenzene-d4	13.853	152	80458	22.643	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.560%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	3381	0.612	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040422\
Data File : VW022391.D
Acq On : 04 Apr 2022 17:05
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK410

Quant Time: Apr 05 01:57:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 05 01:44:25 2022
Response via : Initial Calibration

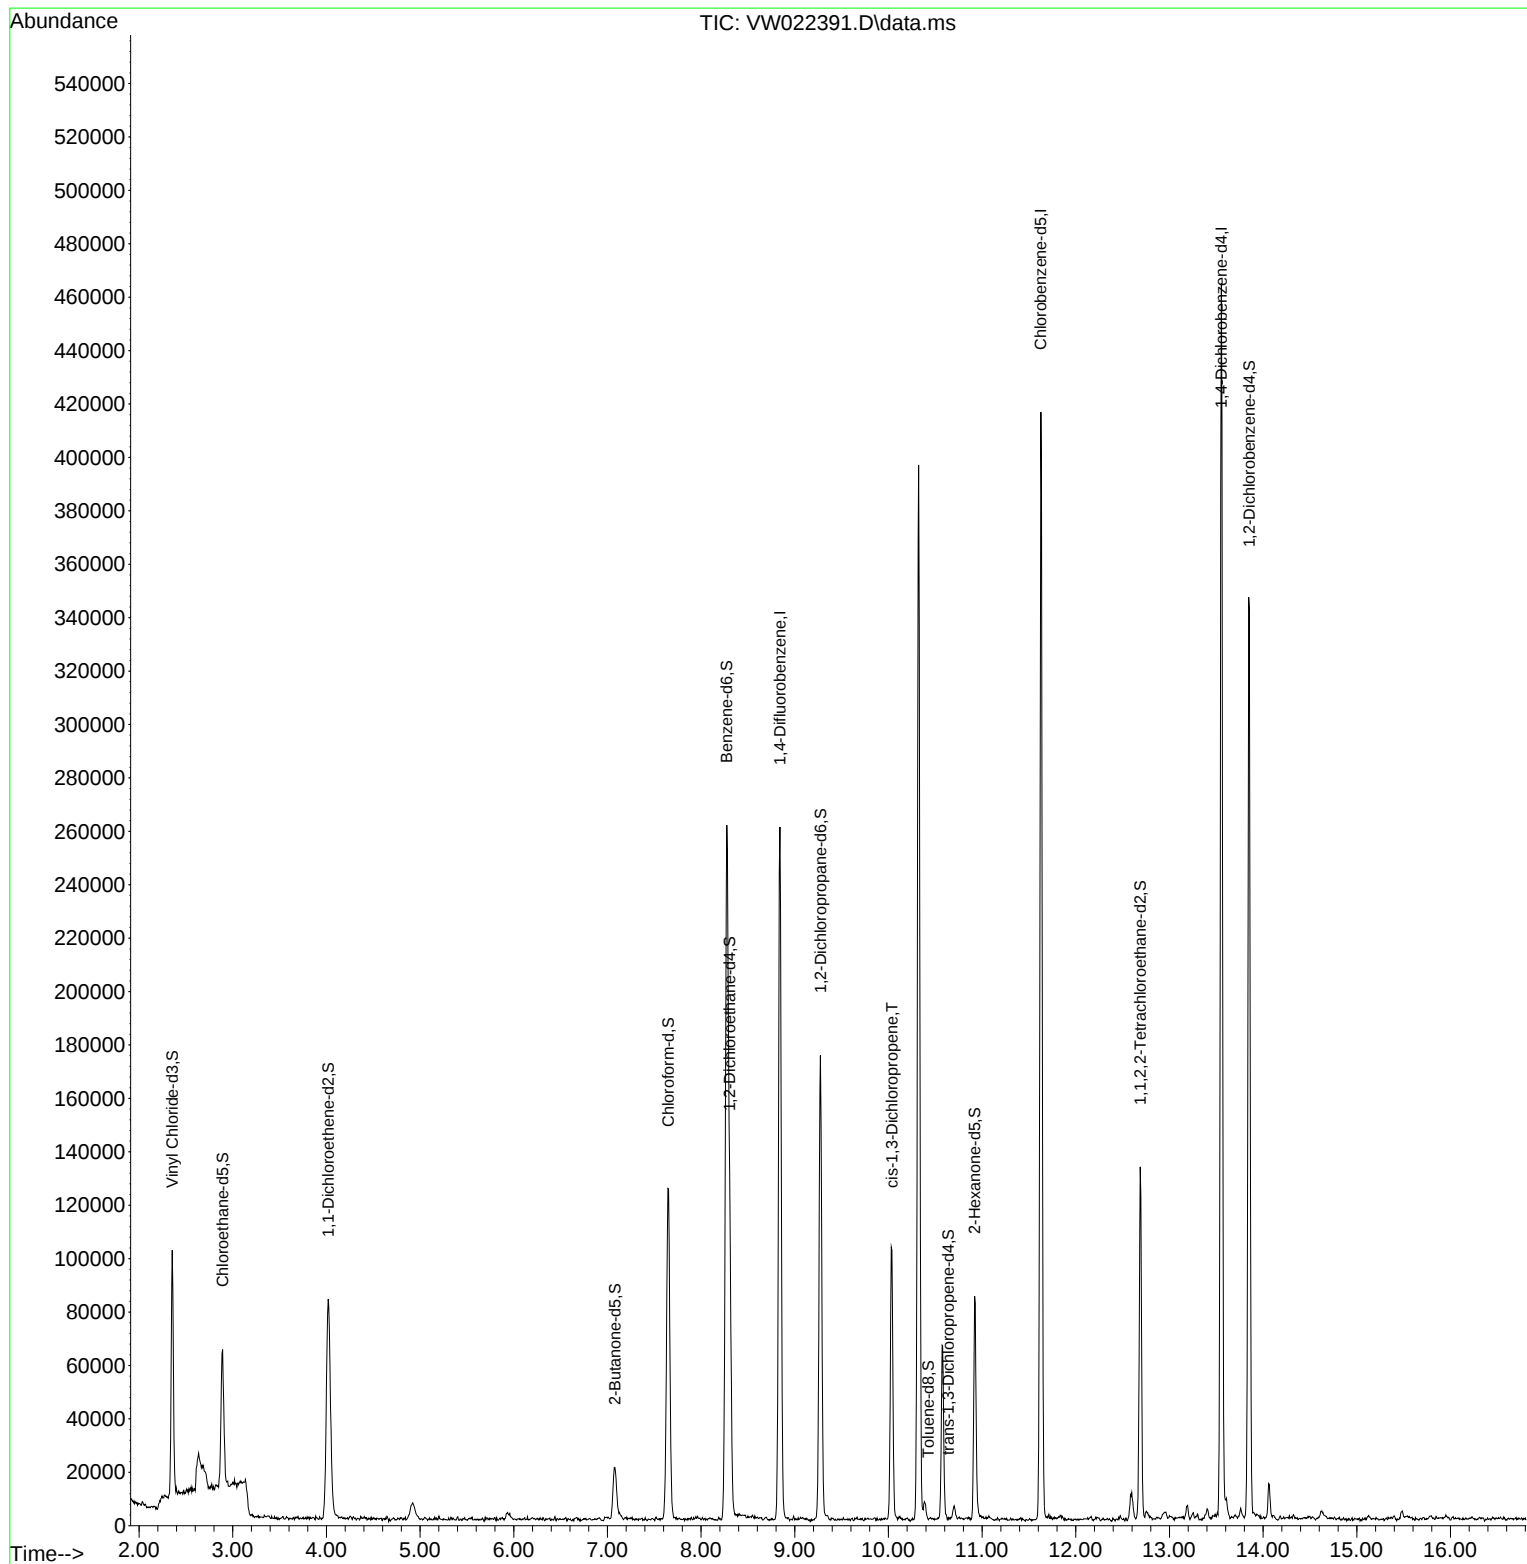

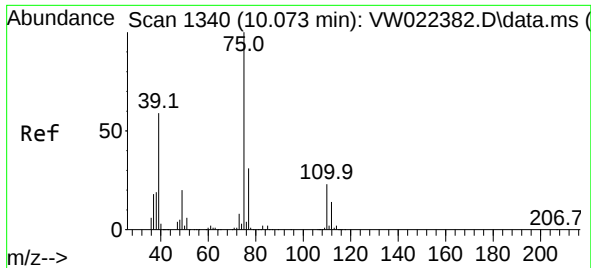

#39

cis-1,3-Dichloropropene

Concen: 0.612 ug/L

RT: 10.036 min Scan# 11

Delta R.T. -0.037 min

Lab File: VW022391.D


Acq: 04 Apr 2022 17:05

Instrument :

MSVOA_W

ClientSampleId :

VIBLK410

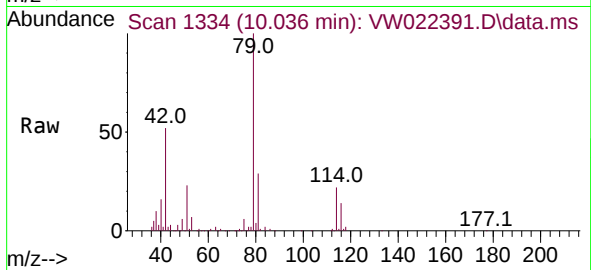

Tgt Ion: 75 Resp: 3381

Ion Ratio Lower Upper

75 100

77 37.3 20.6 38.2

