




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040422\
Data File : VW022386.D
Acq On : 04 Apr 2022 15:04
Operator : SY/VA
Sample : N2225-05
Misc : 7.99g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGQD4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/05/2022
Supervised By :Mahesh Dadoda 04/06/2022

Quant Time: Apr 05 01:56:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 05 01:44:25 2022
Response via : Initial Calibration

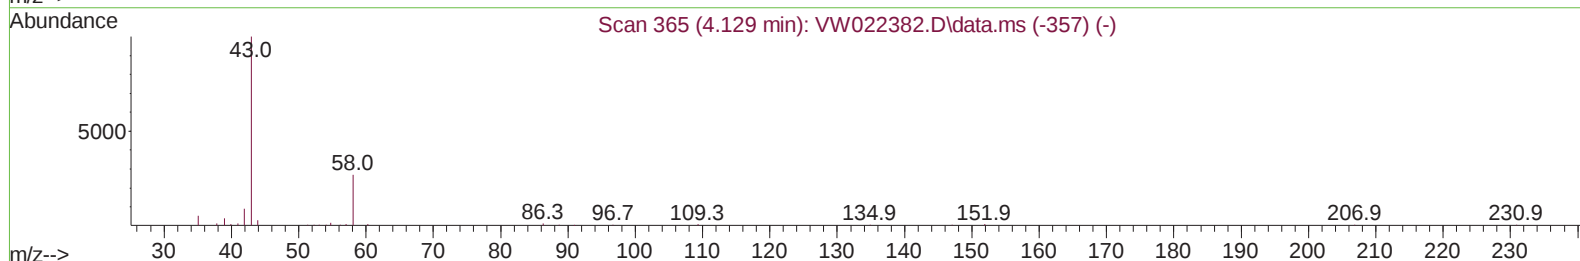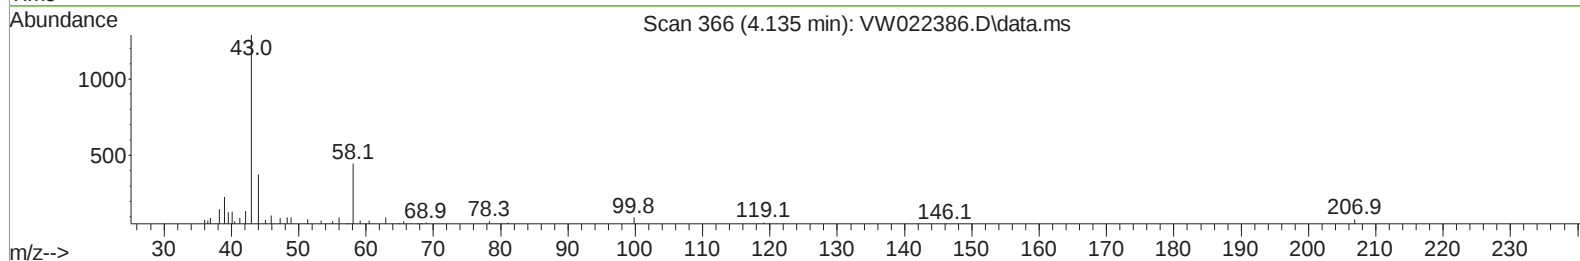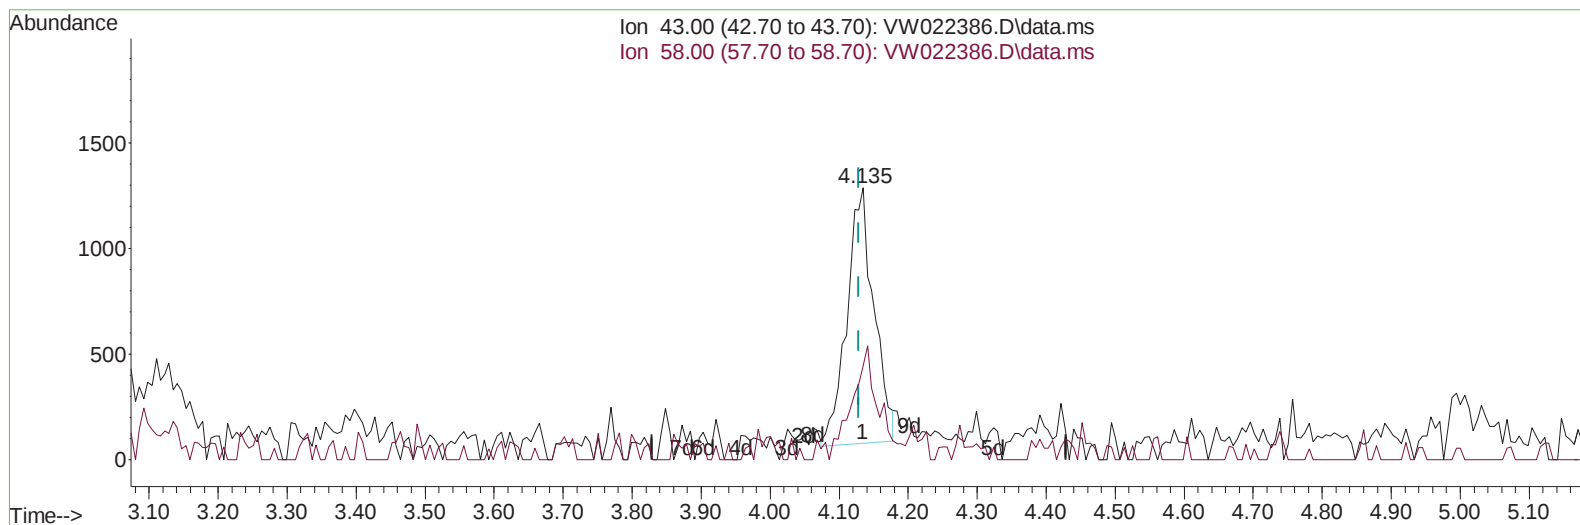

TIC: VW022386.D\data.ms

(13) Acetone (T)

4.135min (+ 0.006) 6.48 ug/L

response 3286

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	36.24
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040422\
 Data File : VW022386.D
 Acq On : 04 Apr 2022 15:04
 Operator : SY/VA
 Sample : N2225-05
 Misc : 7.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQD4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/05/2022
 Supervised By :Mahesh Dadoda 04/06/2022

Quant Time: Apr 05 01:56:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 05 01:44:25 2022
 Response via : Initial Calibration

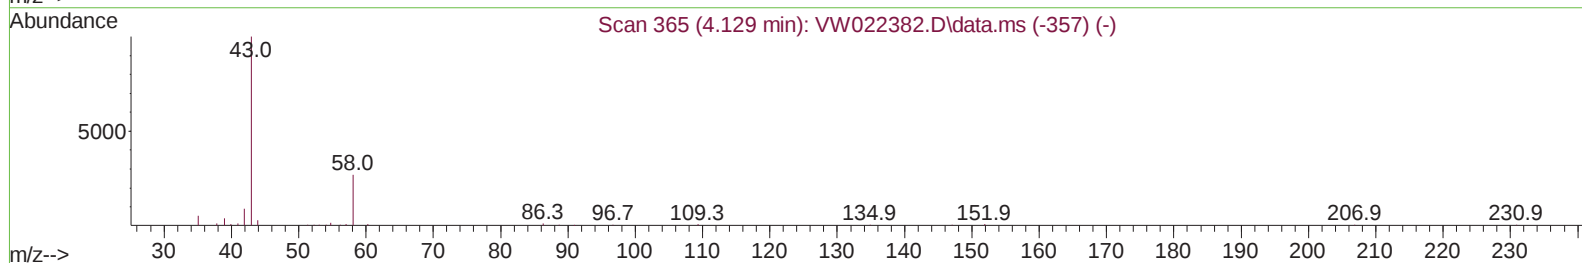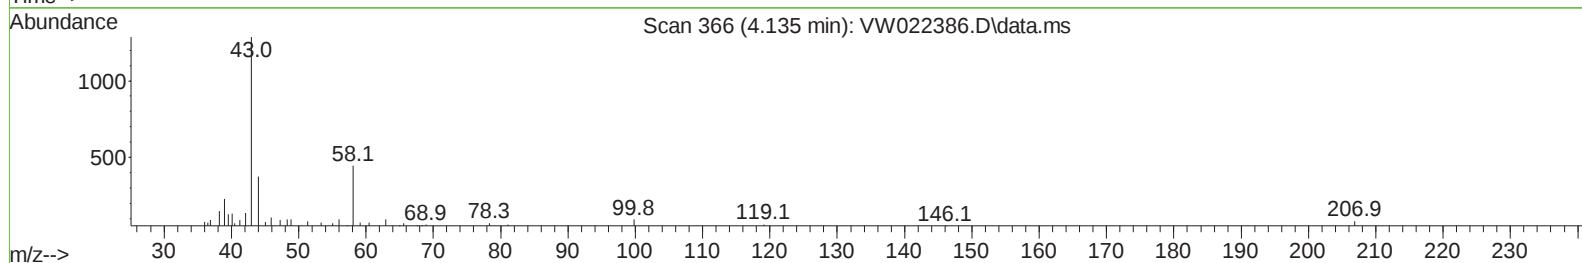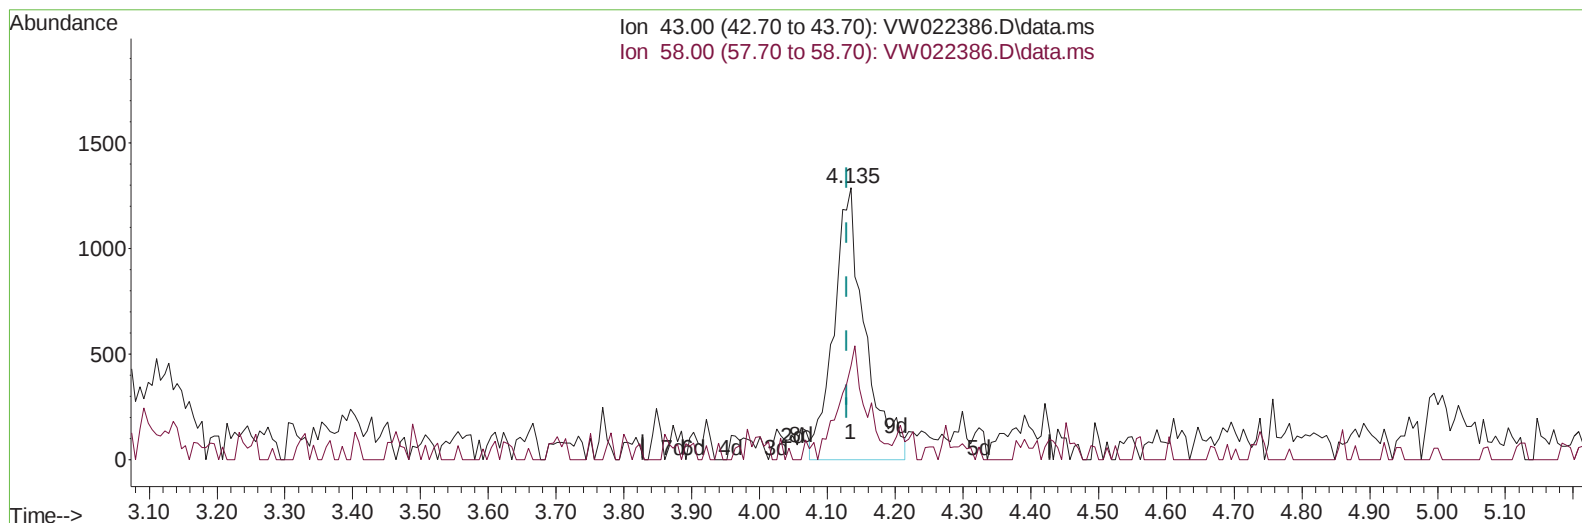

TIC: VW022386.D\data.ms

(13) Acetone (T)

4.135min (+ 0.006) 8.09 ug/L m

response 4099

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	29.06
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040422\
 Data File : VW022386.D
 Acq On : 04 Apr 2022 15:04
 Operator : SY/VA
 Sample : N2225-05
 Misc : 7.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQD4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/05/2022
 Supervised By :Mahesh Dadoda 04/06/2022

Quant Time: Apr 05 01:56:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 05 01:44:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	184856	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	177735	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	93991	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	79760	26.327	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	105.320%	
7) Chloroethane-d5	2.891	69	56557	31.270	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	125.080%	
11) 1,1-Dichloroethene-d2	4.019	63	80455	17.898	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	71.600%	
21) 2-Butanone-d5	7.079	46	50718	68.512	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	137.020%#	
24) Chloroform-d	7.652	84	117349	22.767	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	91.080%	
26) 1,2-Dichloroethane-d4	8.305	65	82421	27.043	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	108.160%	
32) Benzene-d6	8.274	84	245794	25.184	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	100.720%	
36) 1,2-Dichloropropane-d6	9.274	67	73479	25.077	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	100.320%	
41) Toluene-d8	10.323	98	238937	25.732	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	102.920%	
43) trans-1,3-Dichloroprop...	10.579	79	37467	25.428	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	101.720%	
47) 2-Hexanone-d5	10.920	63	41941	69.875	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	139.760%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	77903	31.515	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	126.040%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	84026	27.693	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	110.760%	
Target Compounds						
13) Acetone	4.135	43	4099m	8.086	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040422\
Data File : VW022386.D
Acq On : 04 Apr 2022 15:04
Operator : SY/VA
Sample : N2225-05
Misc : 7.99g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGQD4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/05/2022
Supervised By :Mahesh Dadoda 04/06/2022

Quant Time: Apr 05 01:56:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 05 01:44:25 2022
Response via : Initial Calibration

