




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040422\
Data File : VW022388.D
Acq On : 04 Apr 2022 15:52
Operator : SY/VA
Sample : N2179-01RE
Misc : 3.32g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0R21RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/05/2022
Supervised By :Mahesh Dadoda 04/06/2022

Quant Time: Apr 05 01:56:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 05 01:44:25 2022
Response via : Initial Calibration

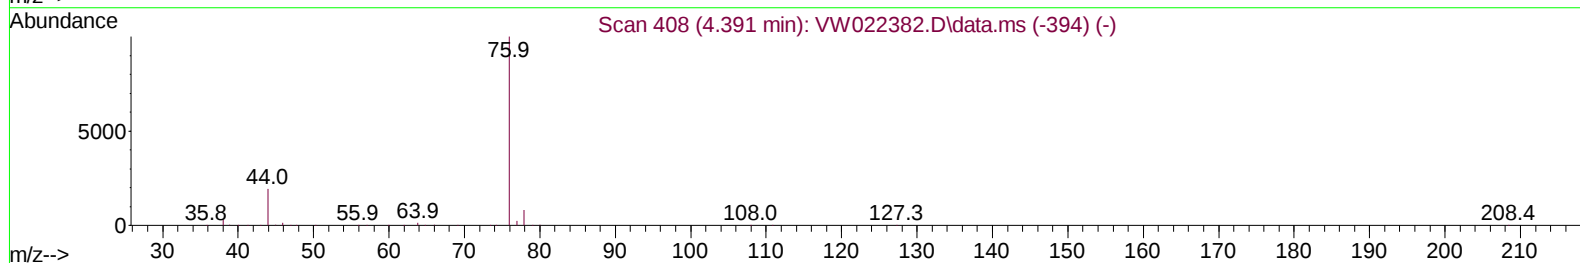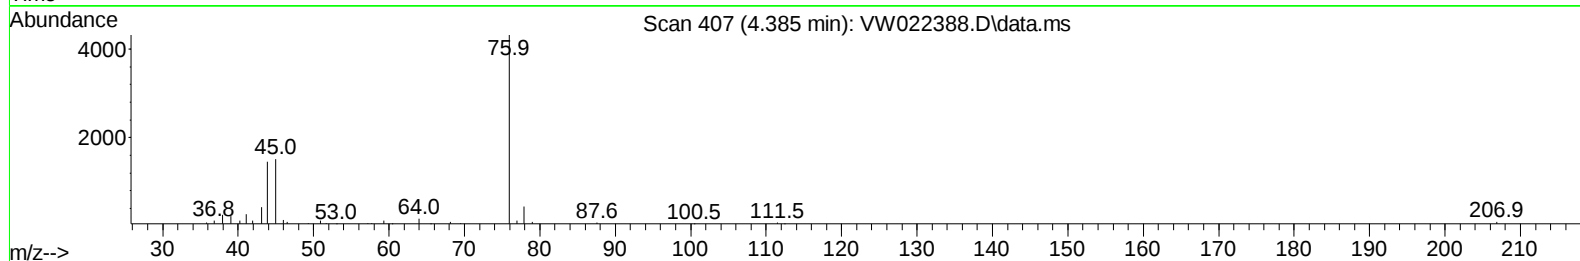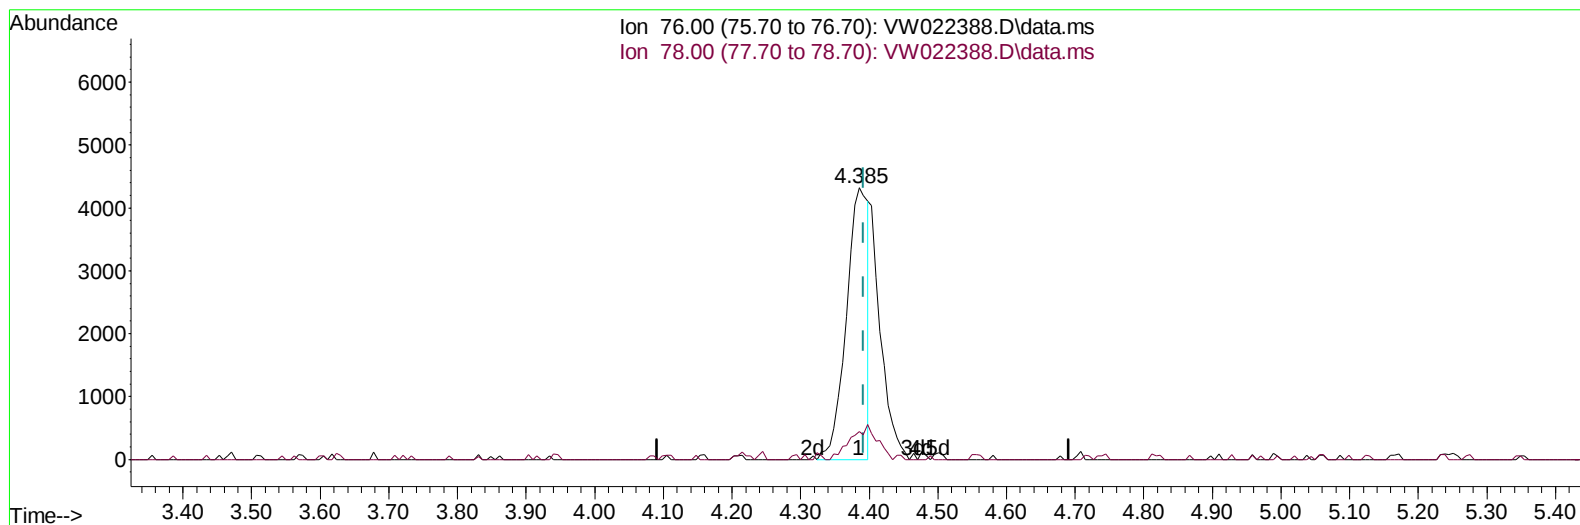

TIC: VW022388.D\data.ms

(14) Carbon disulfide (T)

4.385min (-0.006) 1.21 ug/L

response 9432

Ion	Exp%	Act%
76.00	100.00	100.00
78.00	9.80	10.28
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040422\
 Data File : VW022388.D
 Acq On : 04 Apr 2022 15:52
 Operator : SY/VA
 Sample : N2179-01RE
 Misc : 3.32g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0R21RE

Manual IntegrationsAPPROVED

Quant Time: Apr 05 01:56:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 05 01:44:25 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/05/2022
 Supervised By :Mahesh Dadoda 04/06/2022

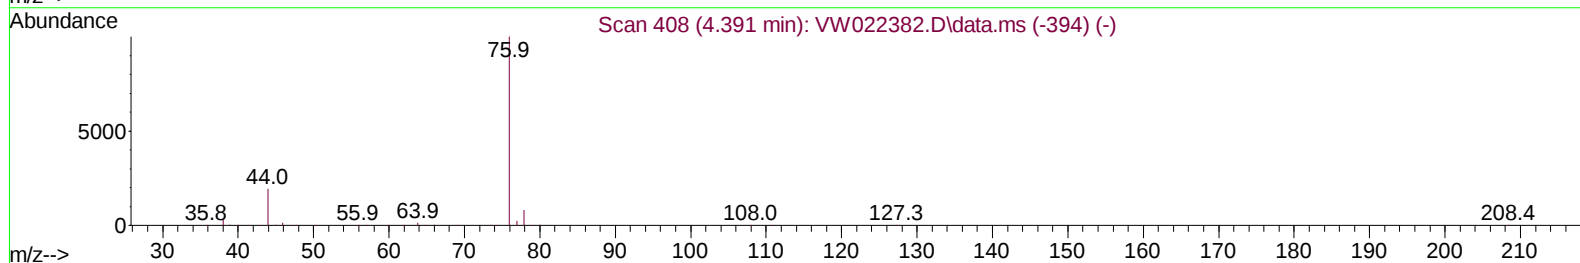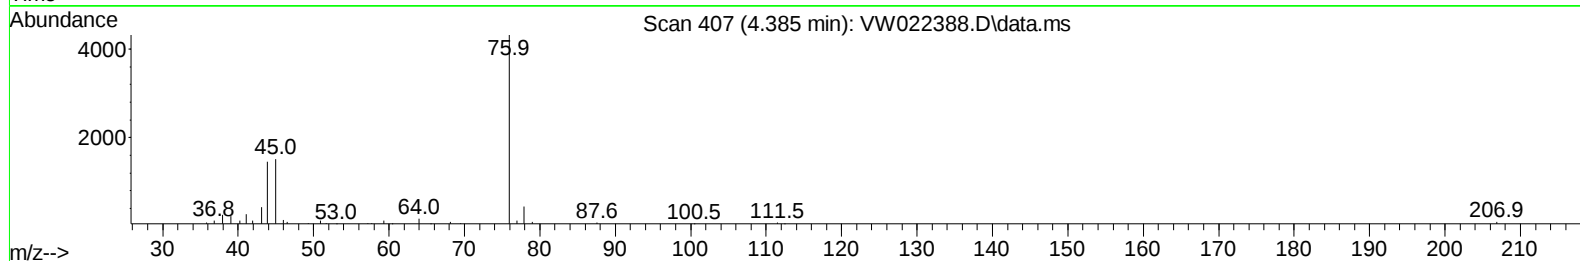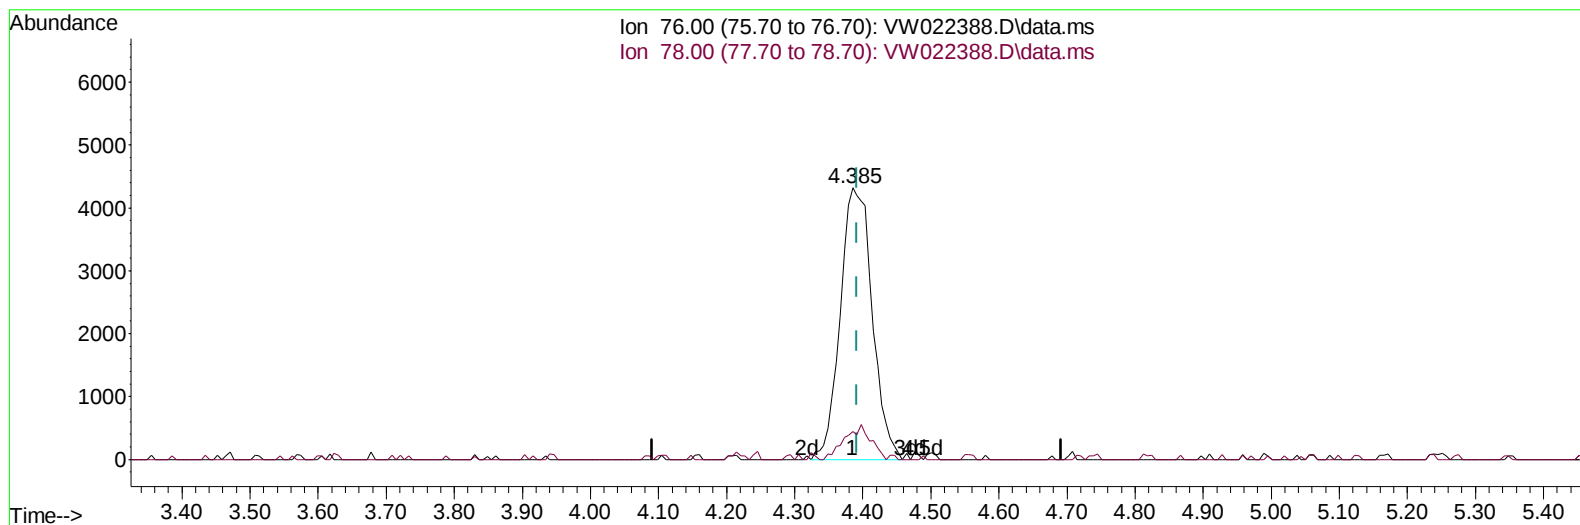

TIC: VW022388.D\data.ms

(14) Carbon disulfide (T)

4.385min (-0.006) 1.79 ug/L m

response 14013

Ion	Exp%	Act%
76.00	100.00	100.00
78.00	9.80	10.28
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040422\
 Data File : VW022388.D
 Acq On : 04 Apr 2022 15:52
 Operator : SY/VA
 Sample : N2179-01RE
 Misc : 3.32g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0R21RE

Manual IntegrationsAPPROVED

Quant Time: Apr 05 01:56:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 05 01:44:25 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/05/2022
 Supervised By :Mahesh Dadoda 04/06/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	196519	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	154627	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	53586	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	98935	30.718	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	122.880%	
7) Chloroethane-d5	2.892	69	69175	35.977	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	143.920%	
11) 1,1-Dichloroethene-d2	4.019	63	88208	18.458	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	73.840%	
21) 2-Butanone-d5	7.080	46	36787	46.744	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	93.480%	
24) Chloroform-d	7.653	84	135756	24.775	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	99.120%	
26) 1,2-Dichloroethane-d4	8.305	65	88165	27.211	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	108.840%	
32) Benzene-d6	8.275	84	283950	33.441	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	133.760%	
36) 1,2-Dichloropropane-d6	9.275	67	82430	32.335	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	129.360%#	
41) Toluene-d8	10.323	98	251844	31.175	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	124.720%	
43) trans-1,3-Dichloroprop...	10.579	79	27270	21.273	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	85.080%	
47) 2-Hexanone-d5	10.921	63	30704	58.799	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	117.600%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	53838	25.034	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	100.120%	
66) 1,2-Dichlorobenzene-d4	13.853	152	46782	27.044	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	108.160%	
Target Compounds						
						Qvalue
13) Acetone	4.123	43	93802	174.061	ug/L	90
14) Carbon disulfide	4.385	76	14013m	1.794	ug/L	
22) 2-Butanone	7.171	43	45188	53.160	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040422\
Data File : VW022388.D
Acq On : 04 Apr 2022 15:52
Operator : SY/VA
Sample : N2179-01RE
Misc : 3.32g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0R21RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/05/2022
Supervised By :Mahesh Dadoda 04/06/2022

Quant Time: Apr 05 01:56:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 05 01:44:25 2022
Response via : Initial Calibration

